Dose-volume histogram — Lung_Patient_19

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

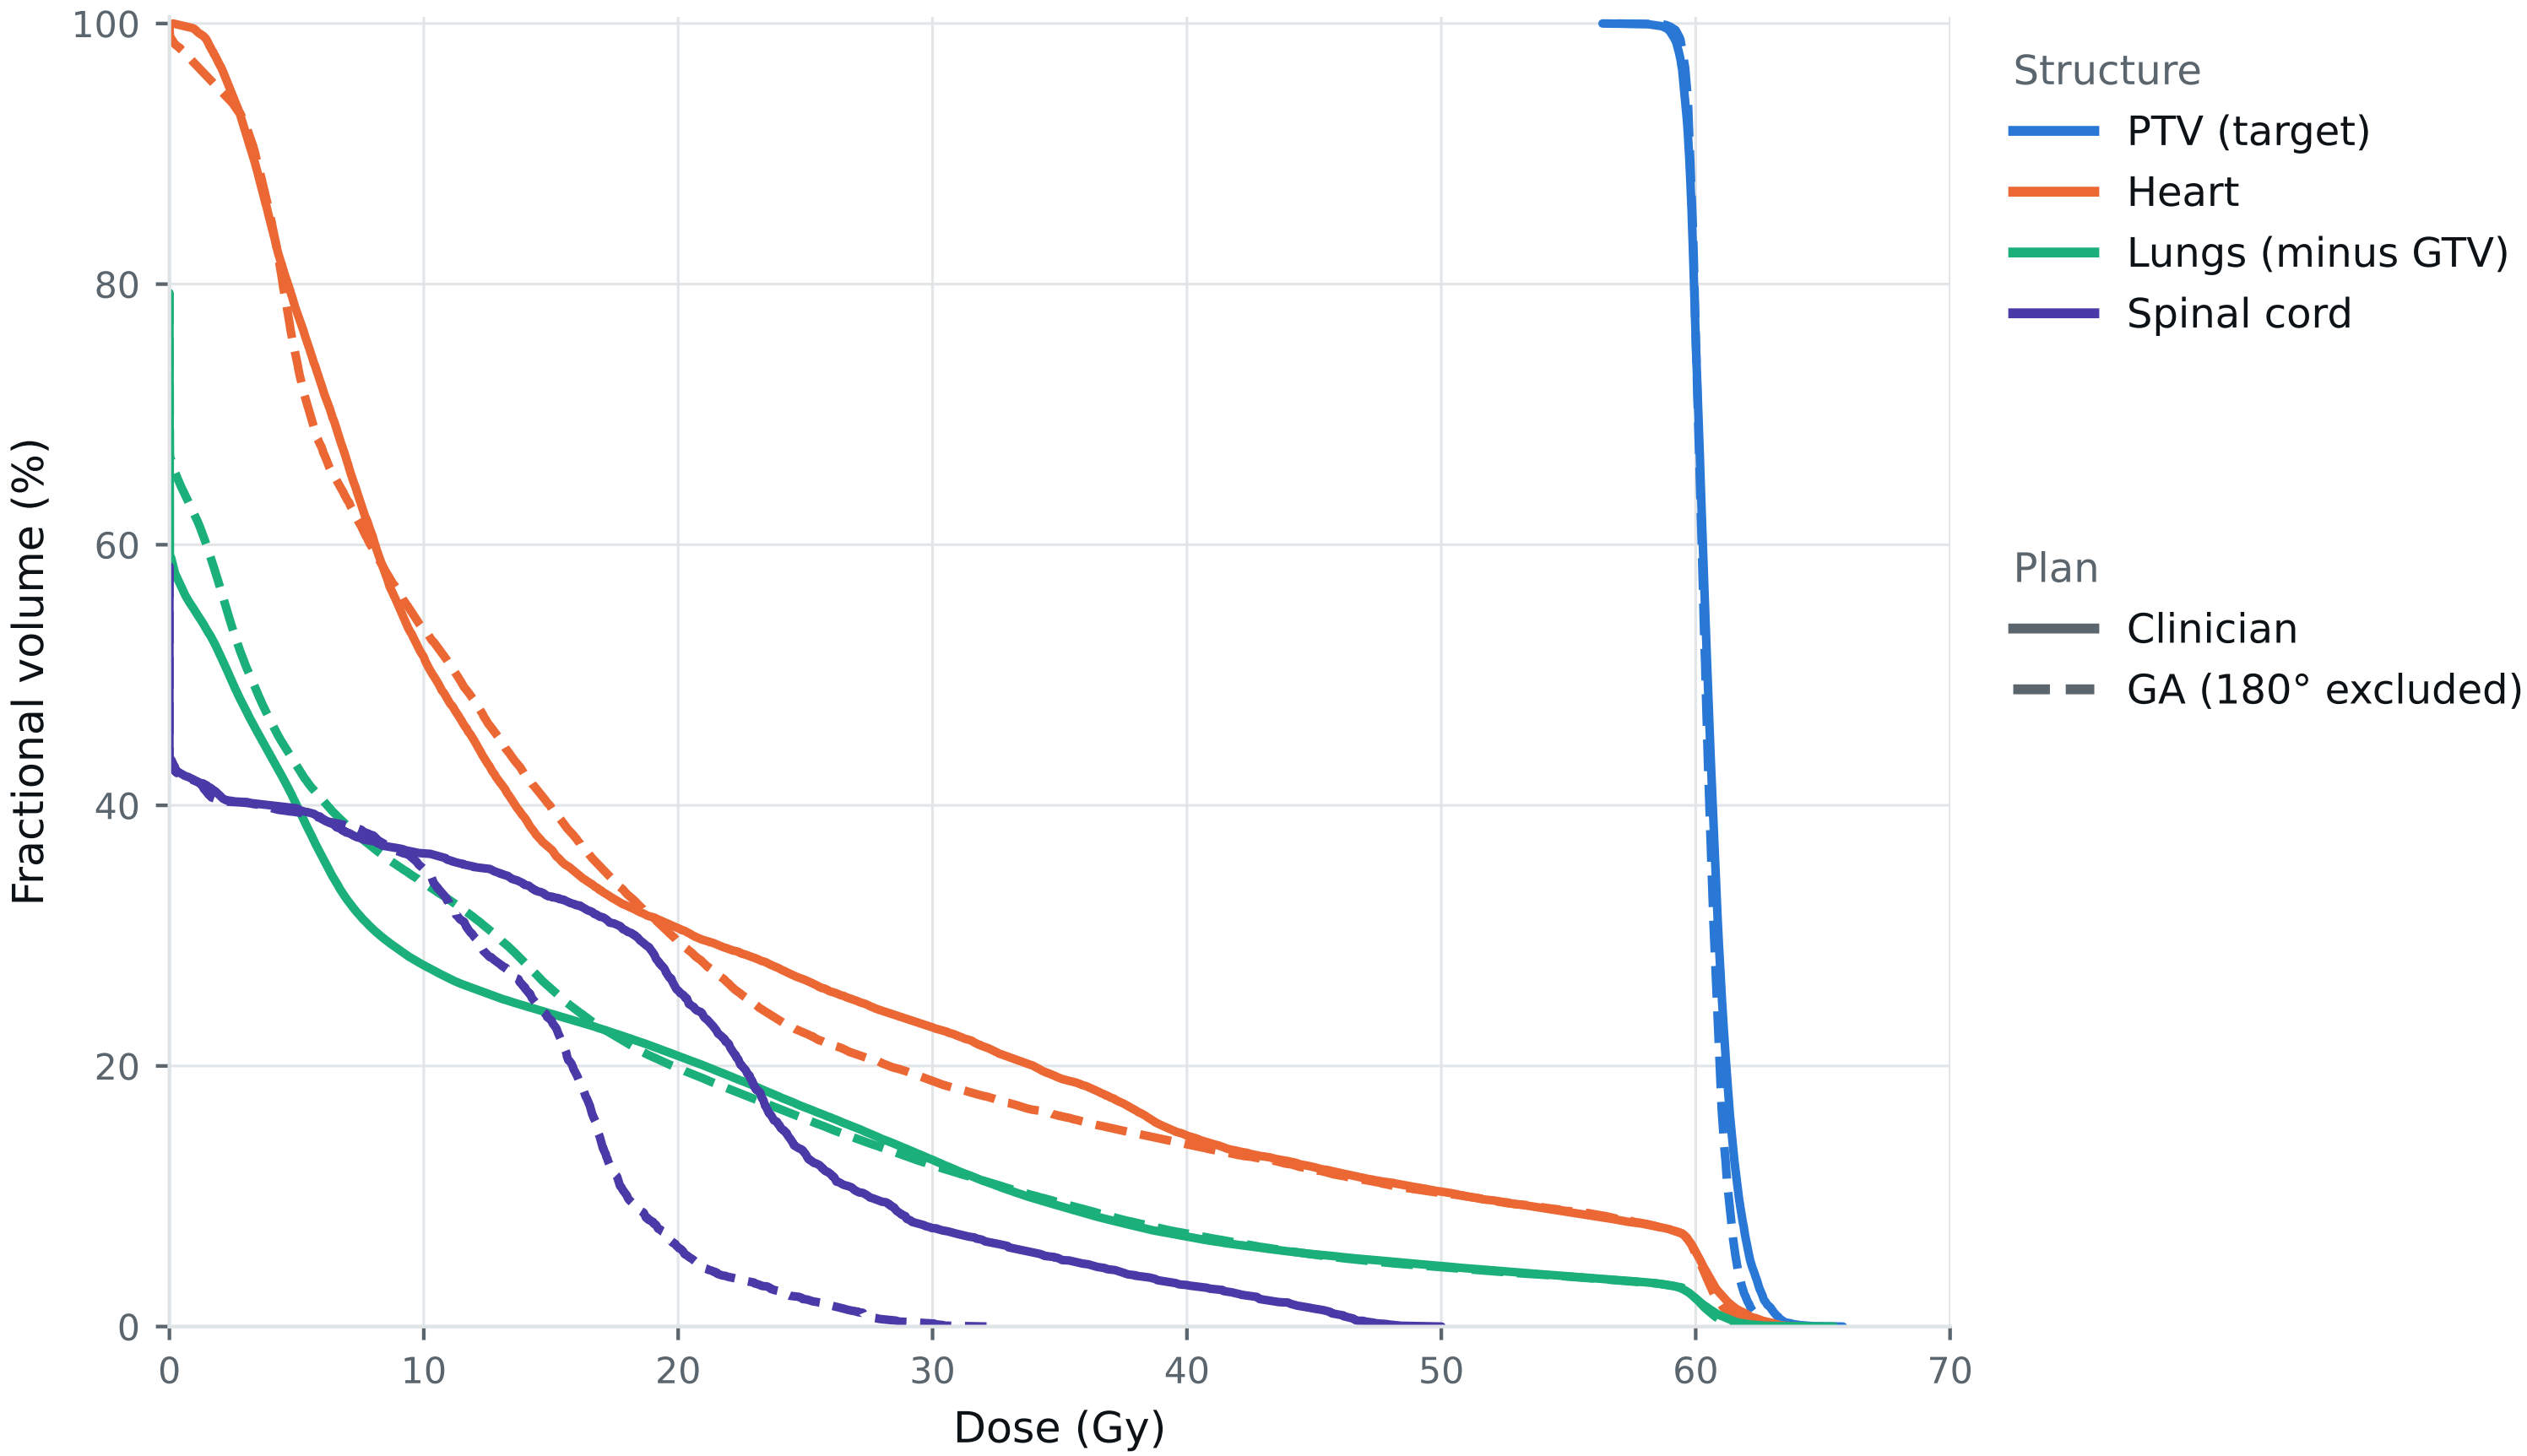

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_19

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

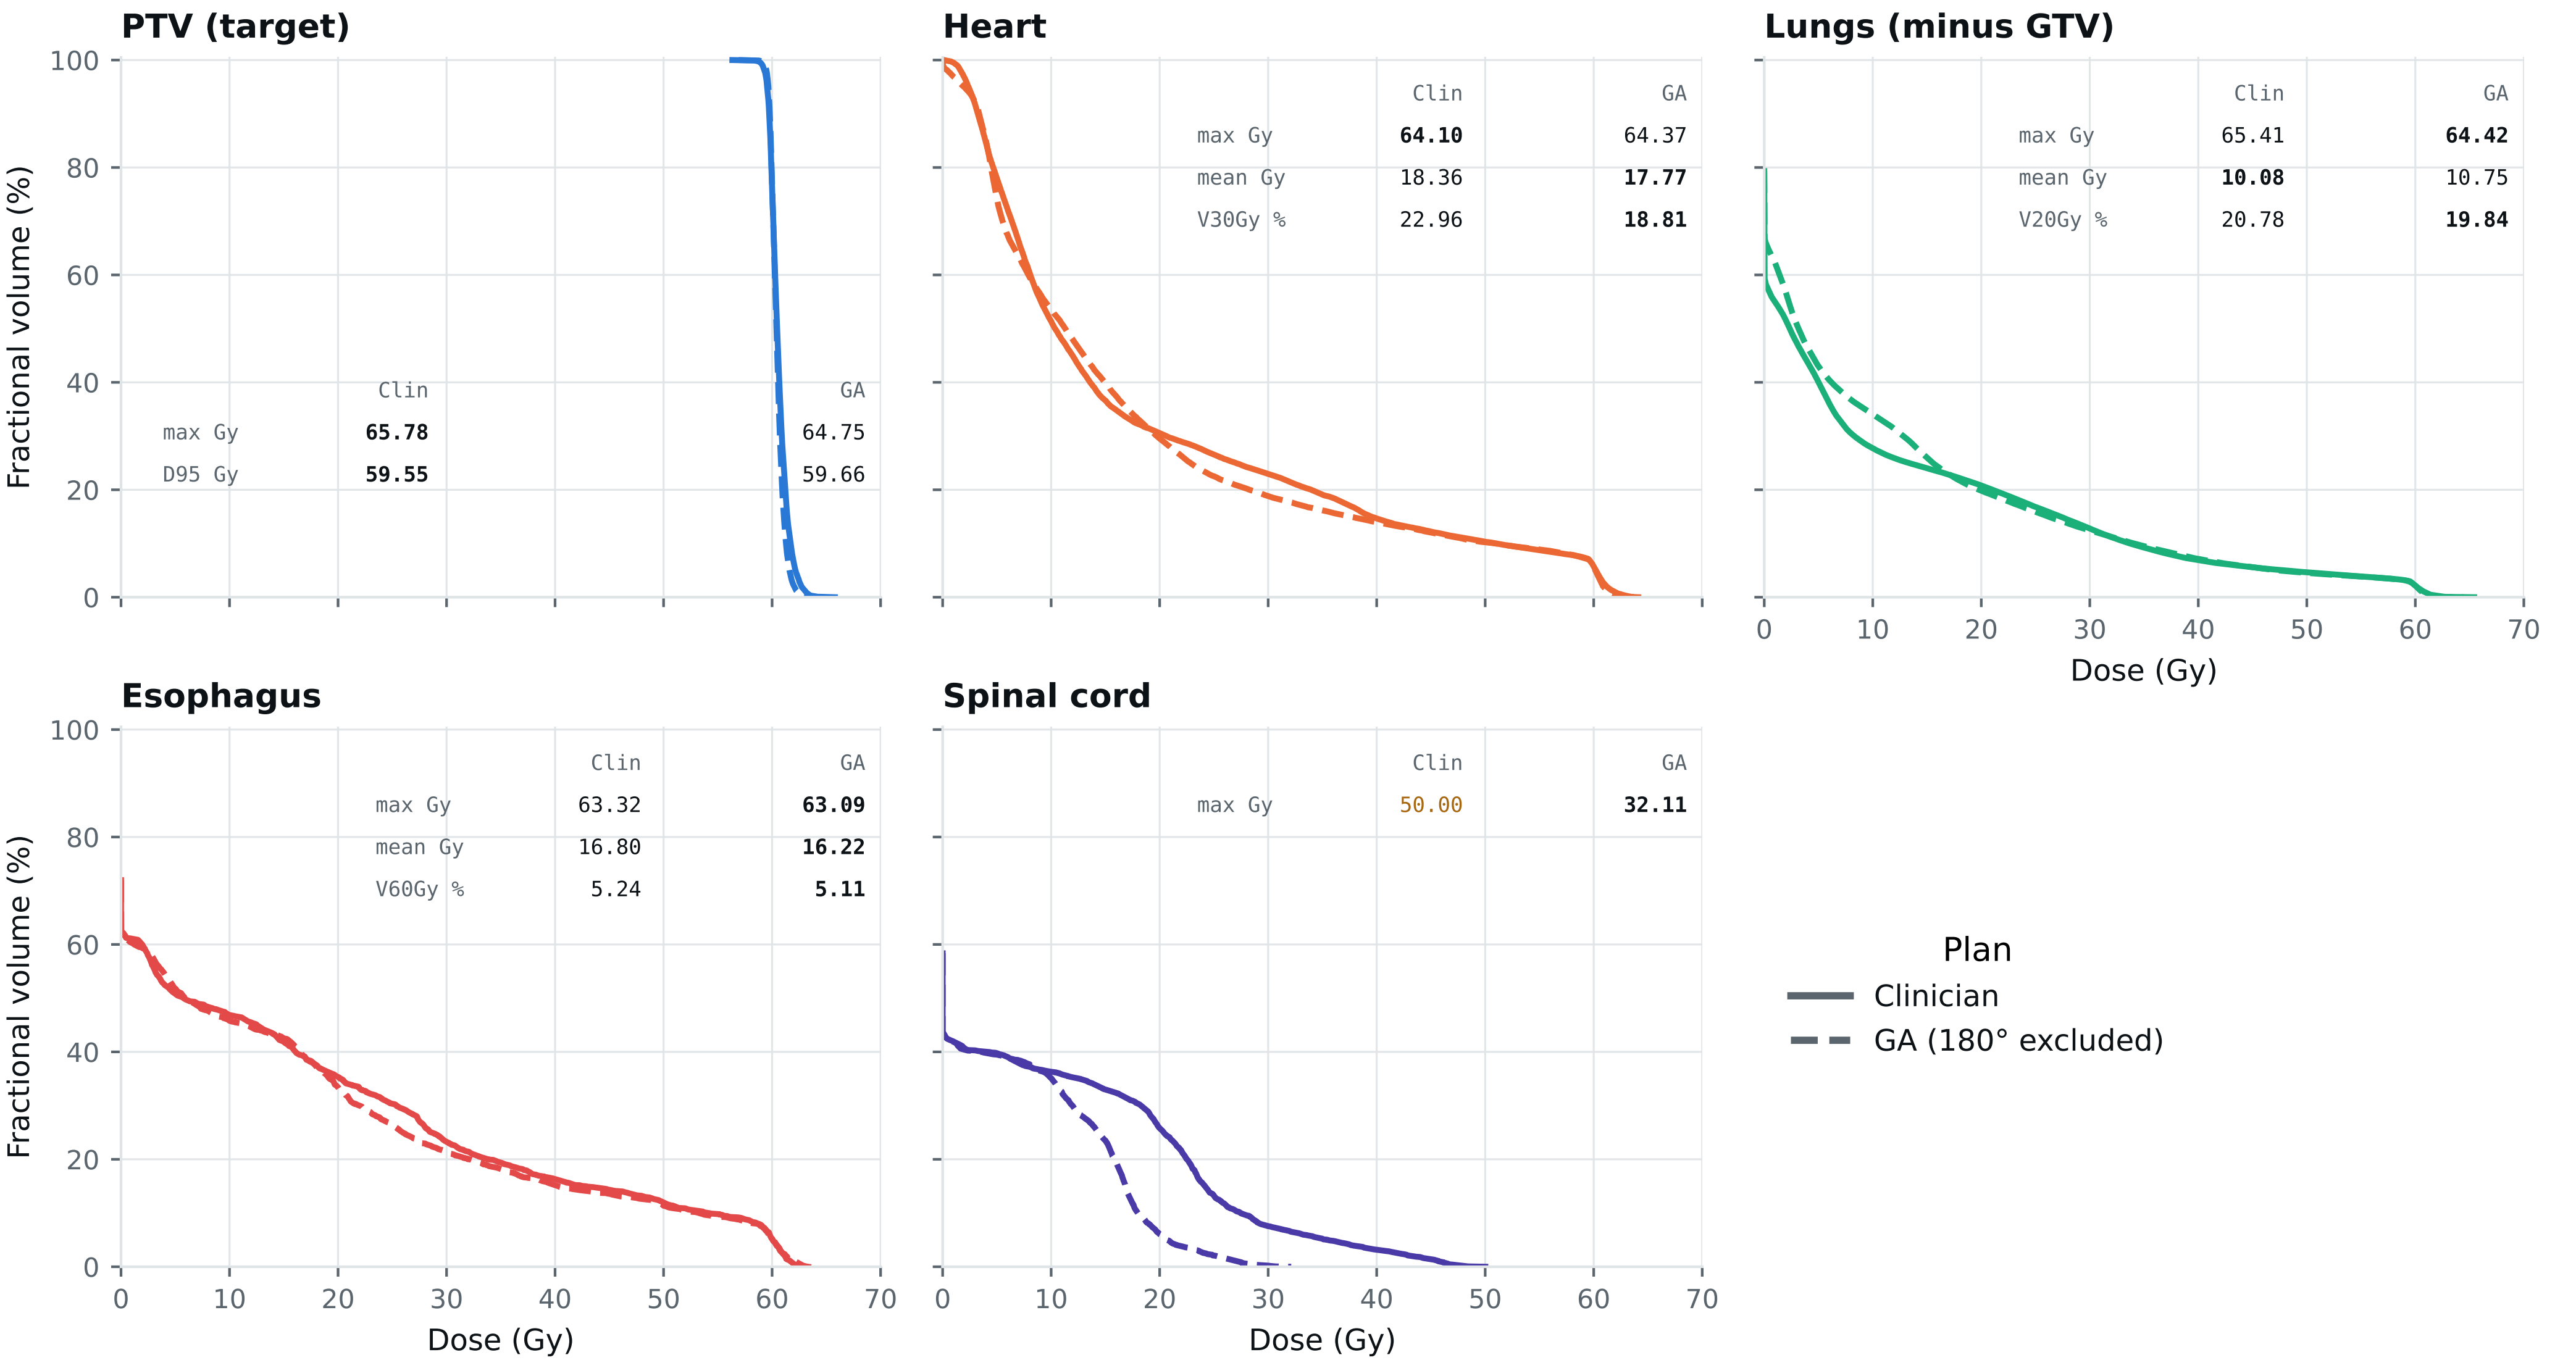

Clinical criteria — Lung_Patient_19

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	63.77	**62.83**	Gy
PTV max	69	66	**65.78**	64.75	Gy
ESOPHAGUS max	66	–	63.32	**63.09**	Gy
ESOPHAGUS mean	34	21	16.80	**16.22**	Gy
ESOPHAGUS V60Gy	17	–	5.24	**5.11**	%
HEART max	66	–	**64.10**	64.37	Gy
HEART mean	27	20	18.36	**17.77**	Gy
HEART V30Gy	50	48	22.96	**18.81**	%
LUNG_L max	66	–	**60.60**	61.10	Gy
LUNG_R max	66	–	65.41	**64.42**	Gy
CORD max	50	48	50.00	**32.11**	Gy
SKIN max	60	–	44.33	**43.23**	Gy
LUNGS_NOT_GTV max	66	–	65.41	**64.42**	Gy
LUNGS_NOT_GTV mean	21	20	**10.08**	10.75	Gy
LUNGS_NOT_GTV V20Gy	37	–	20.78	**19.84**	%
PTV D95 (target coverage)			59.55	59.66	
Objective value (search signal)			107.47	95.39	
Solve time			42 s	45 s	

```
Beam angles (gantry°)   Clinician  0°, 335°, 305°, 238°, 212°, 185°
                        GA         212°, 185°, 15°, 105°, 255°, 315°, 345°
```

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_19_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.