Dose-volume histogram — Lung_Patient_34

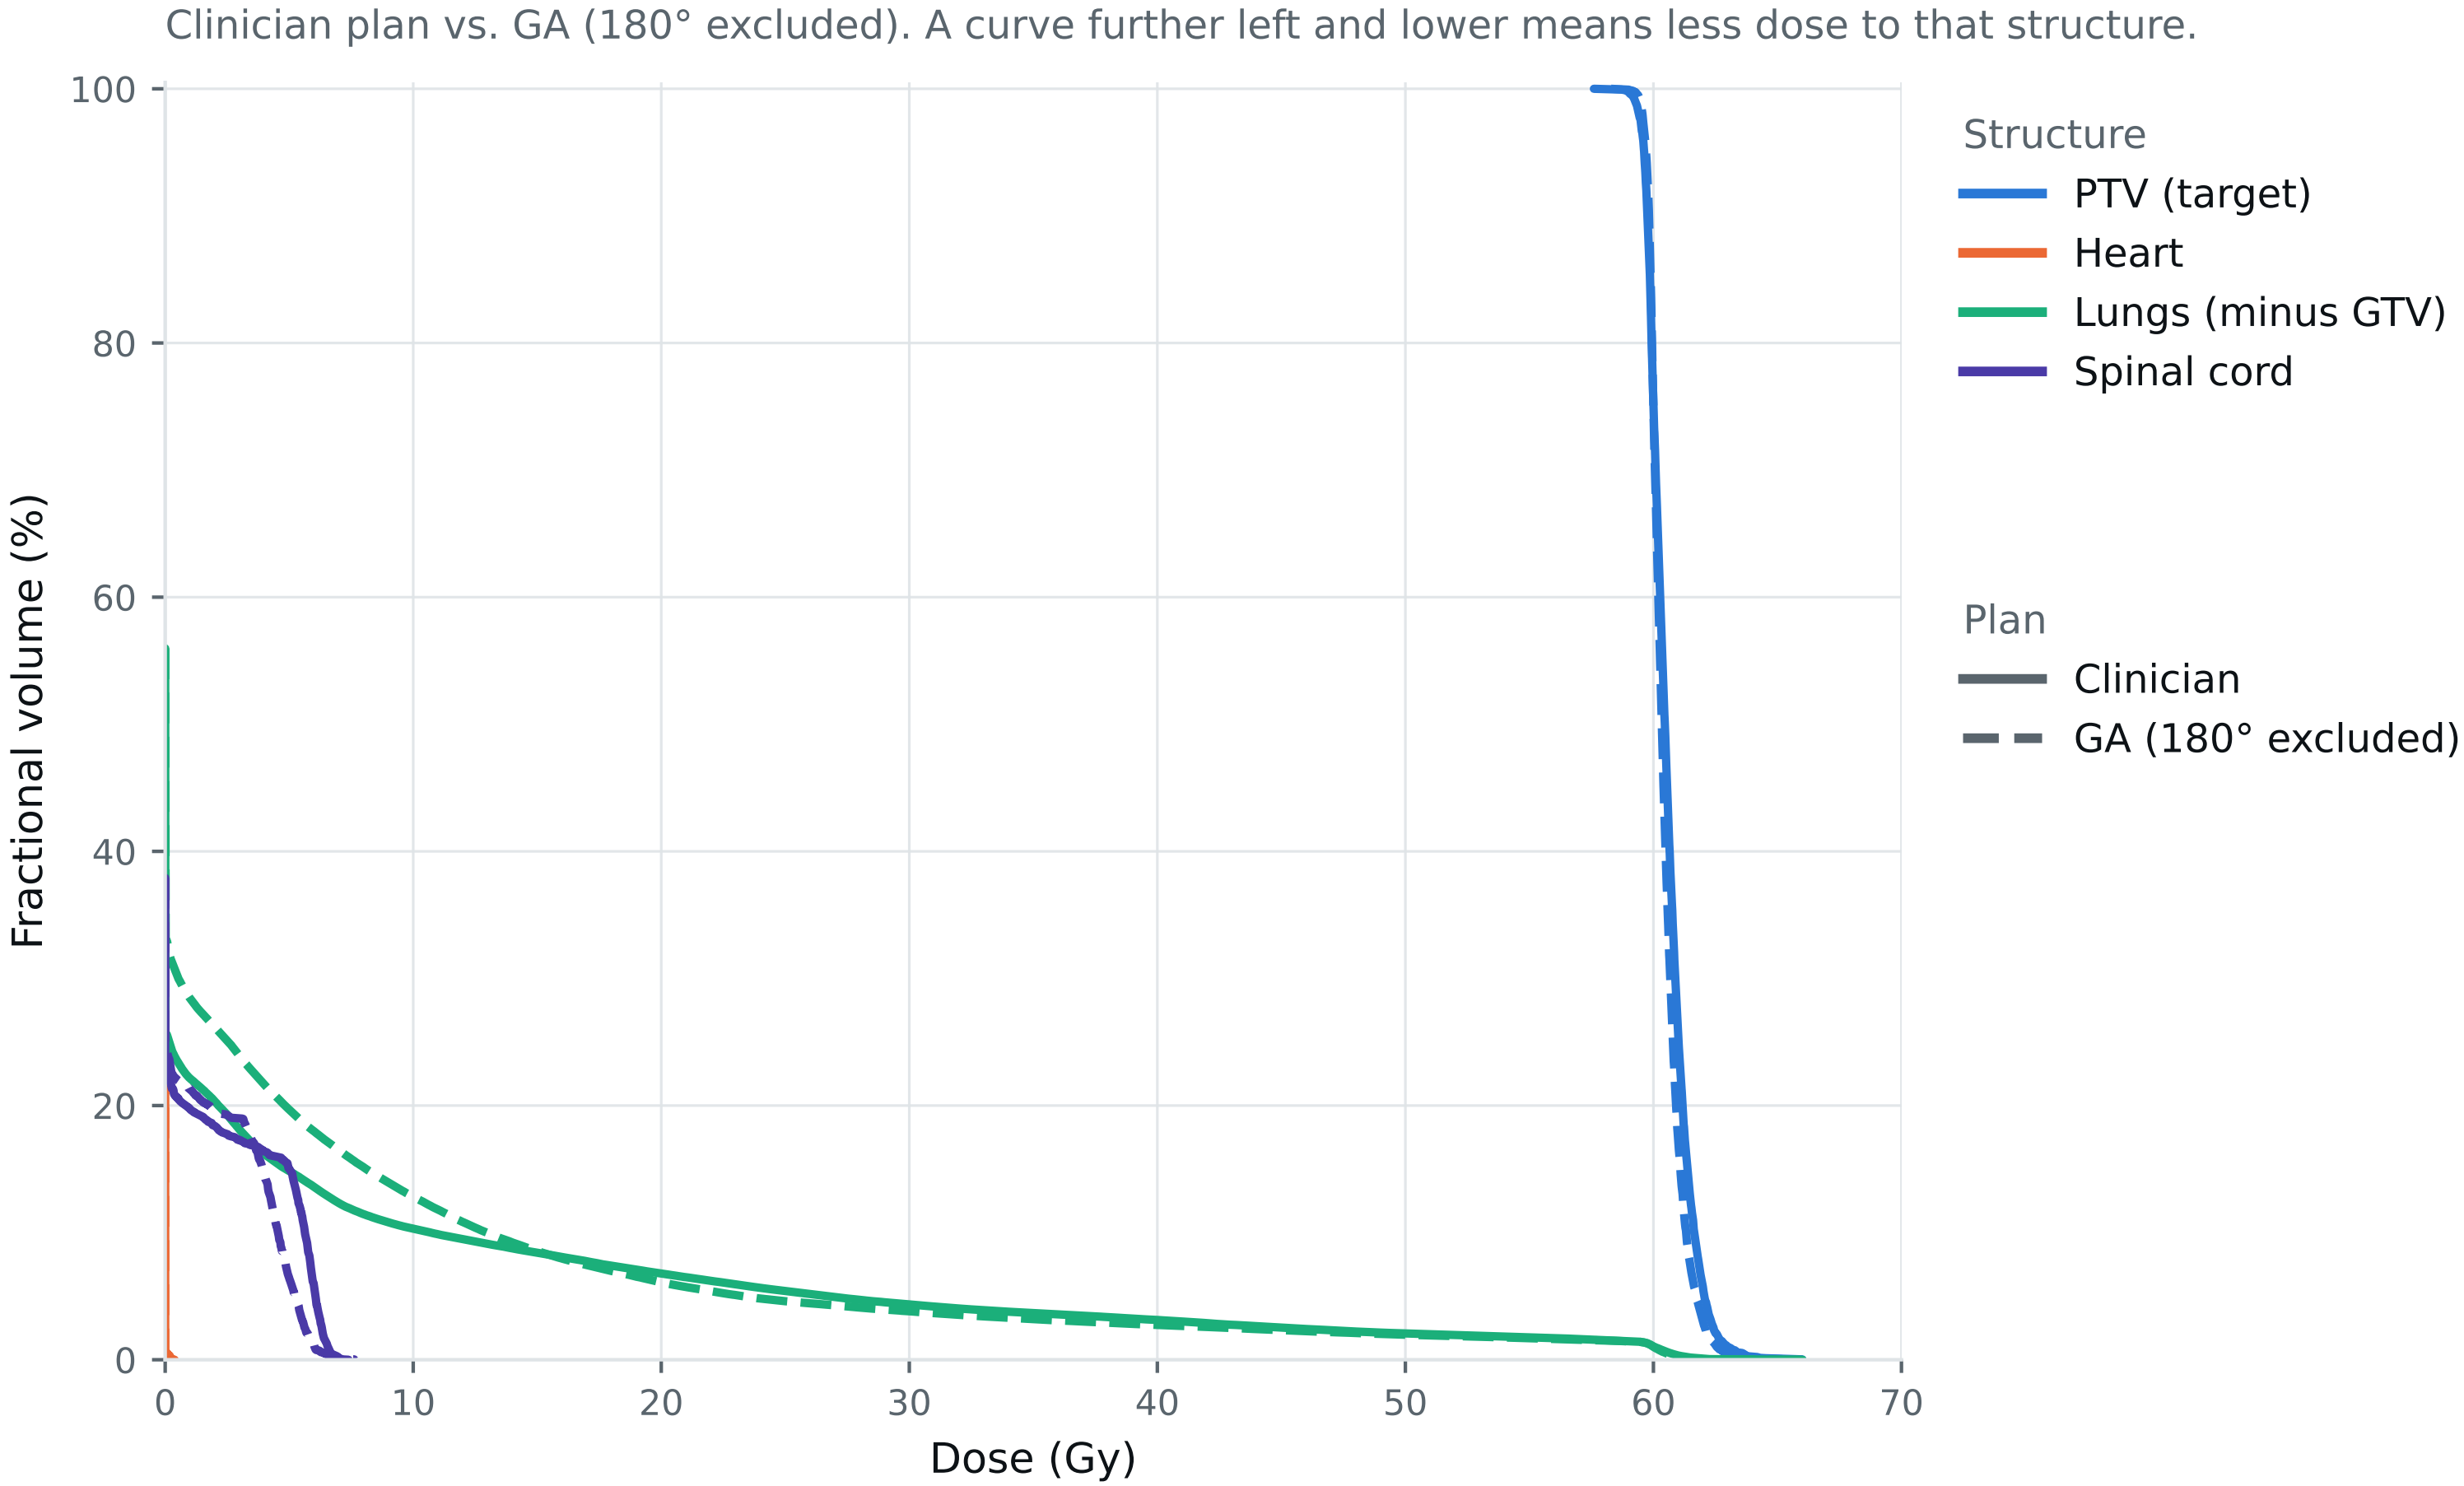

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_34

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

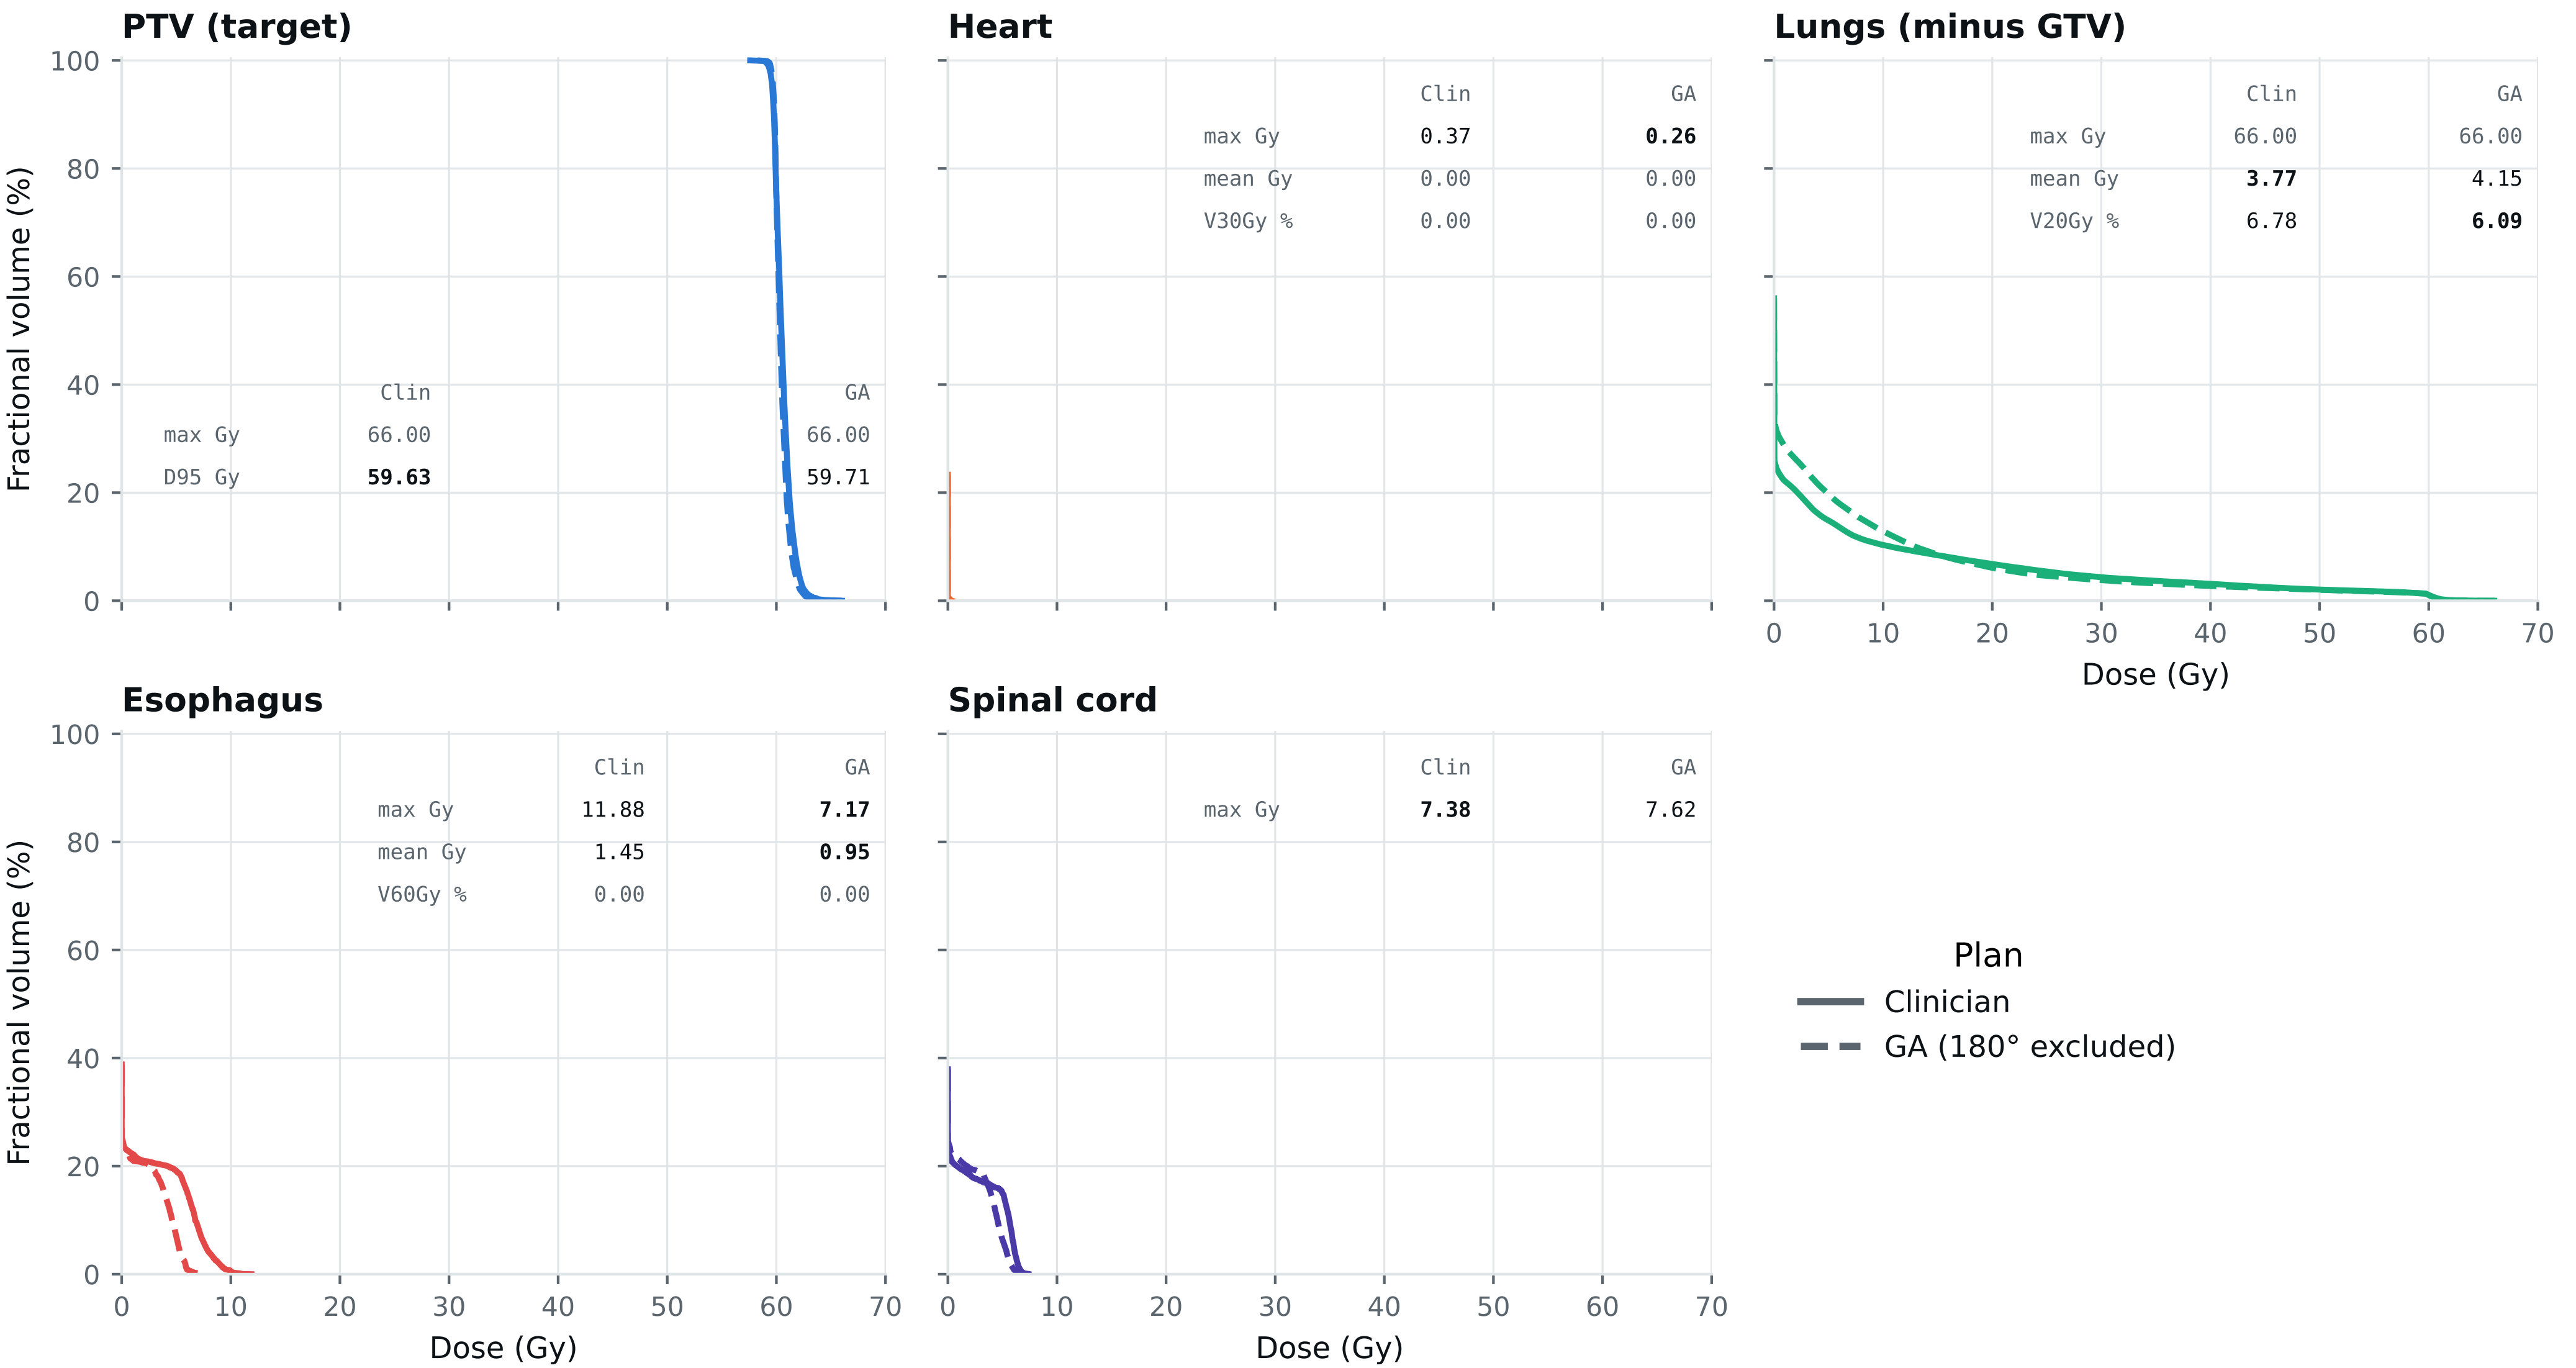

Clinical criteria — Lung_Patient_34

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	64.26	**63.93**	Gy
PTV max	69	66	66.00	66.00	Gy
ESOPHAGUS max	66	–	11.88	**7.17**	Gy
ESOPHAGUS mean	34	21	1.45	**0.95**	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	0.37	**0.26**	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	–	66.00	66.00	Gy
LUNG_R max	66	–	**10.31**	28.23	Gy
CORD max	50	48	**7.38**	7.62	Gy
SKIN max	60	–	42.65	**41.48**	Gy
LUNGS_NOT_GTV max	66	–	66.00	66.00	Gy
LUNGS_NOT_GTV mean	21	20	**3.77**	4.15	Gy
LUNGS_NOT_GTV V20Gy	37	–	6.78	**6.09**	%
PTV D95 (target coverage)			59.63	59.71	
Objective value (search signal)			51.85	43.81	
MOSEK solve time			13 s	13 s	

Beam angles (gantry°)	Clinician	175°, 153°, 130°, 60°, 30°, 0°, 320°
	GA	0°, 15°, 45°, 90°, 120°, 255°, 345°

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_34_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.