Dose-volume histogram — Lung_Patient_15

Clinician plan vs. GA (180° excluded). A curve further left and lower means less dose to that structure.

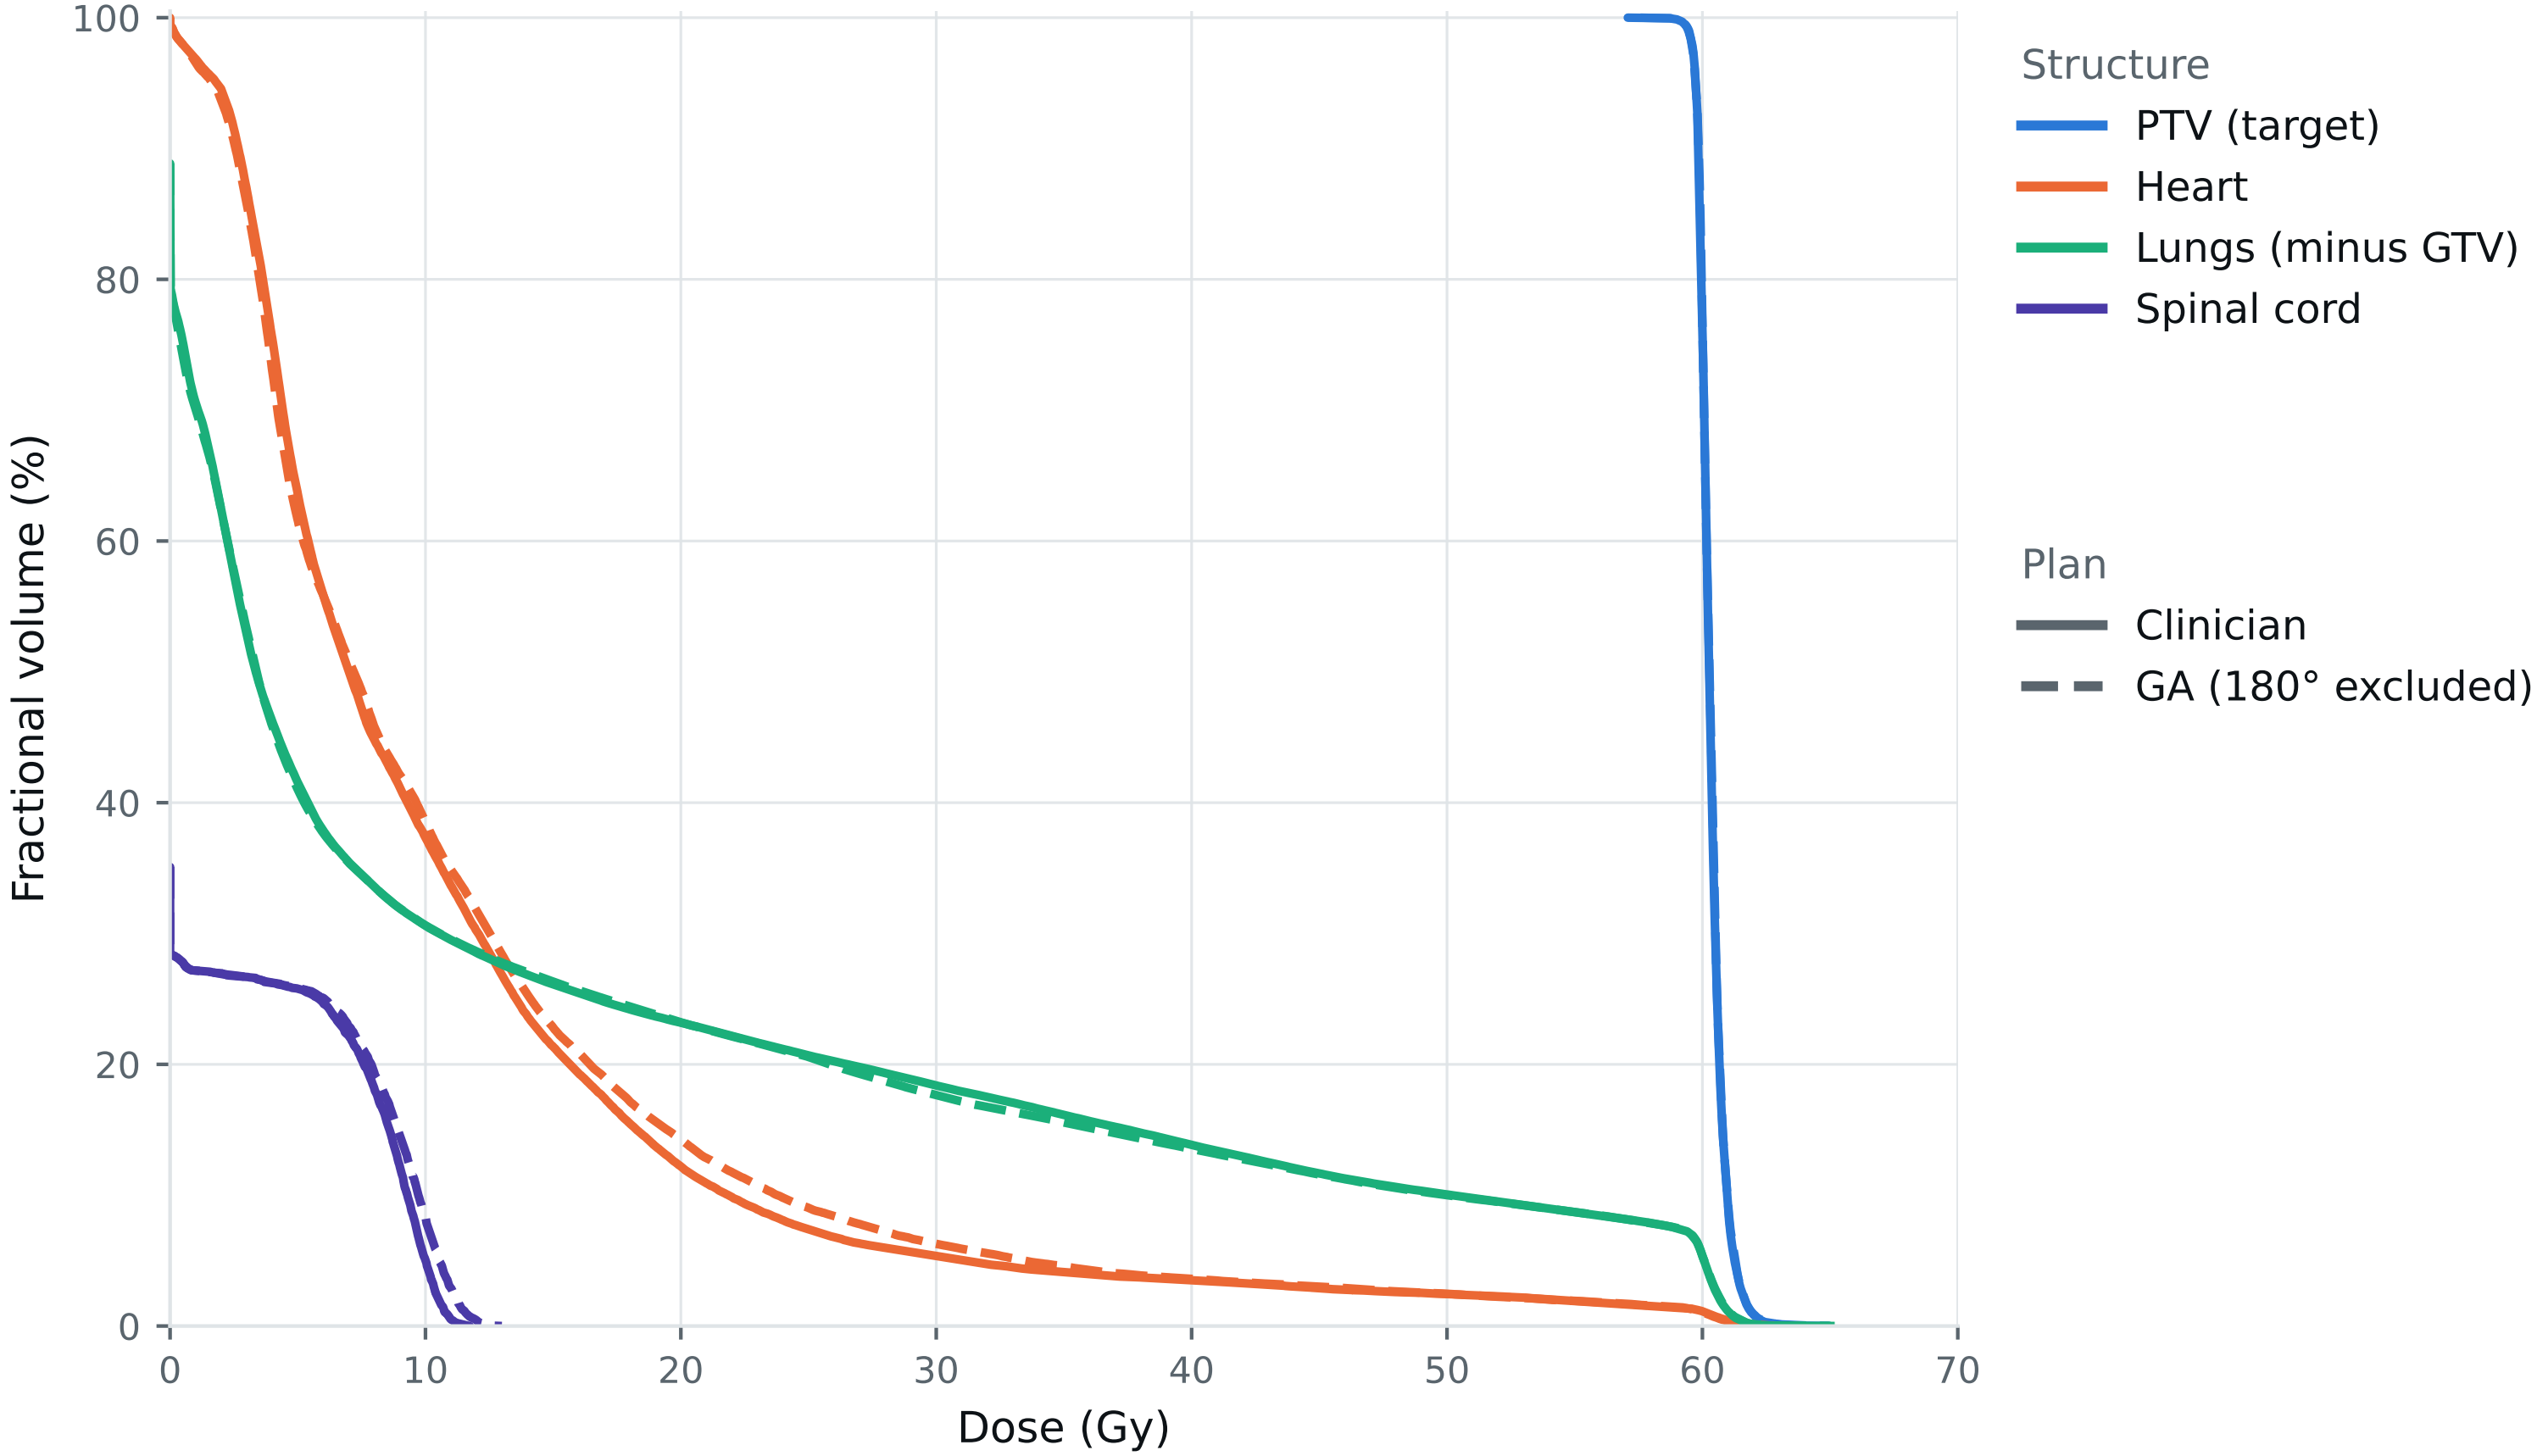

Curves further left are better for organs; the PTV curve should stay high, then drop sharply.
Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_15

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

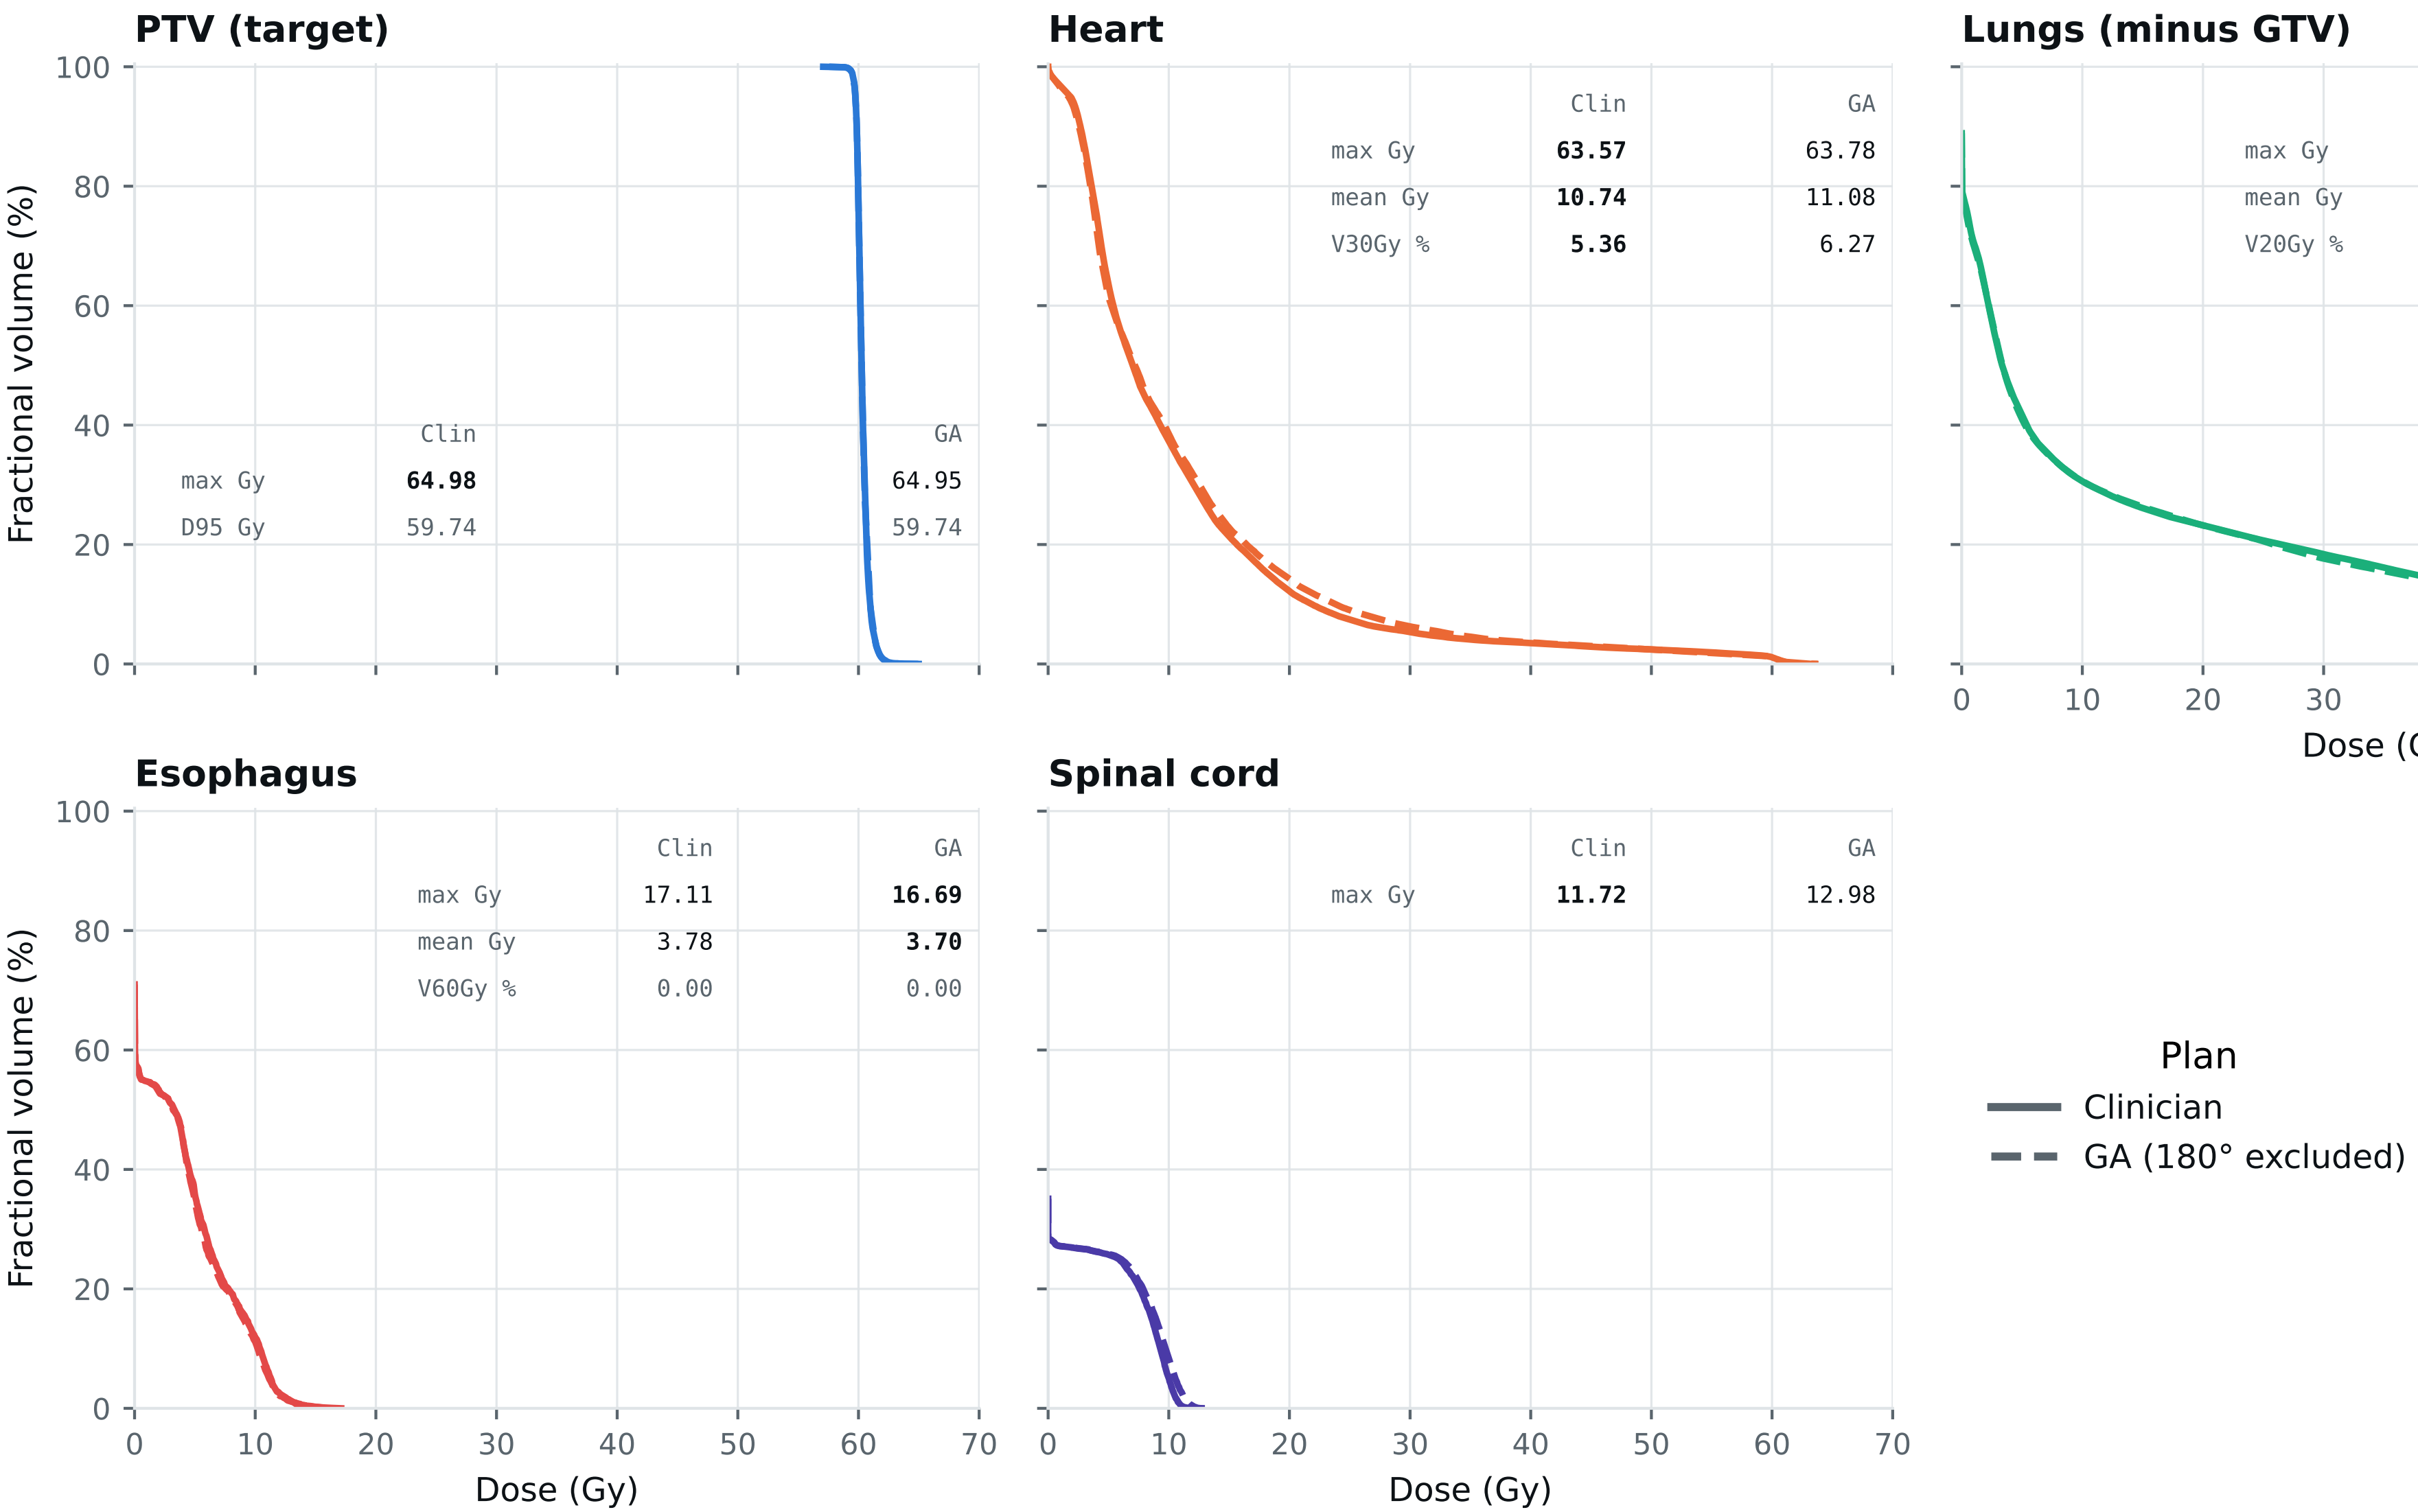

Clinical criteria — Lung_Patient_15

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	**62.20**	62.82	Gy
PTV max	69	66	**64.98**	64.95	Gy
ESOPHAGUS max	66	–	17.11	**16.69**	Gy
ESOPHAGUS mean	34	21	3.78	**3.70**	Gy
ESOPHAGUS V60Gy	17	–	0.00	0.00	%
HEART max	66	–	**63.57**	63.78	Gy
HEART mean	27	20	**10.74**	11.08	Gy
HEART V30Gy	50	48	**5.36**	6.27	%
LUNG_L max	66	–	27.82	**27.45**	Gy
LUNG_R max	66	–	**64.98**	65.17	Gy
CORD max	50	48	**11.72**	12.98	Gy
SKIN max	60	–	60.00	60.00	Gy
LUNGS_NOT_GTV max	66	–	**64.98**	65.17	Gy
LUNGS_NOT_GTV mean	21	20	13.07	**12.97**	Gy
LUNGS_NOT_GTV V20Gy	37	–	**23.19**	23.21	%
PTV D95 (target coverage)			59.74	59.74	
Objective value (search signal)			64.36	64.59	
Pipeline time (setup + solve)			144 s	144 s	

Beam angles (gantry°)		
	Clinician	0°, 330°, 300°, 270°, 240°, 210°, 185°
	GA	0°, 330°, 300°, 270°, 240°, 210°, 15°

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_15_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.