



Dose-volume histogram — Lung_Patient_32

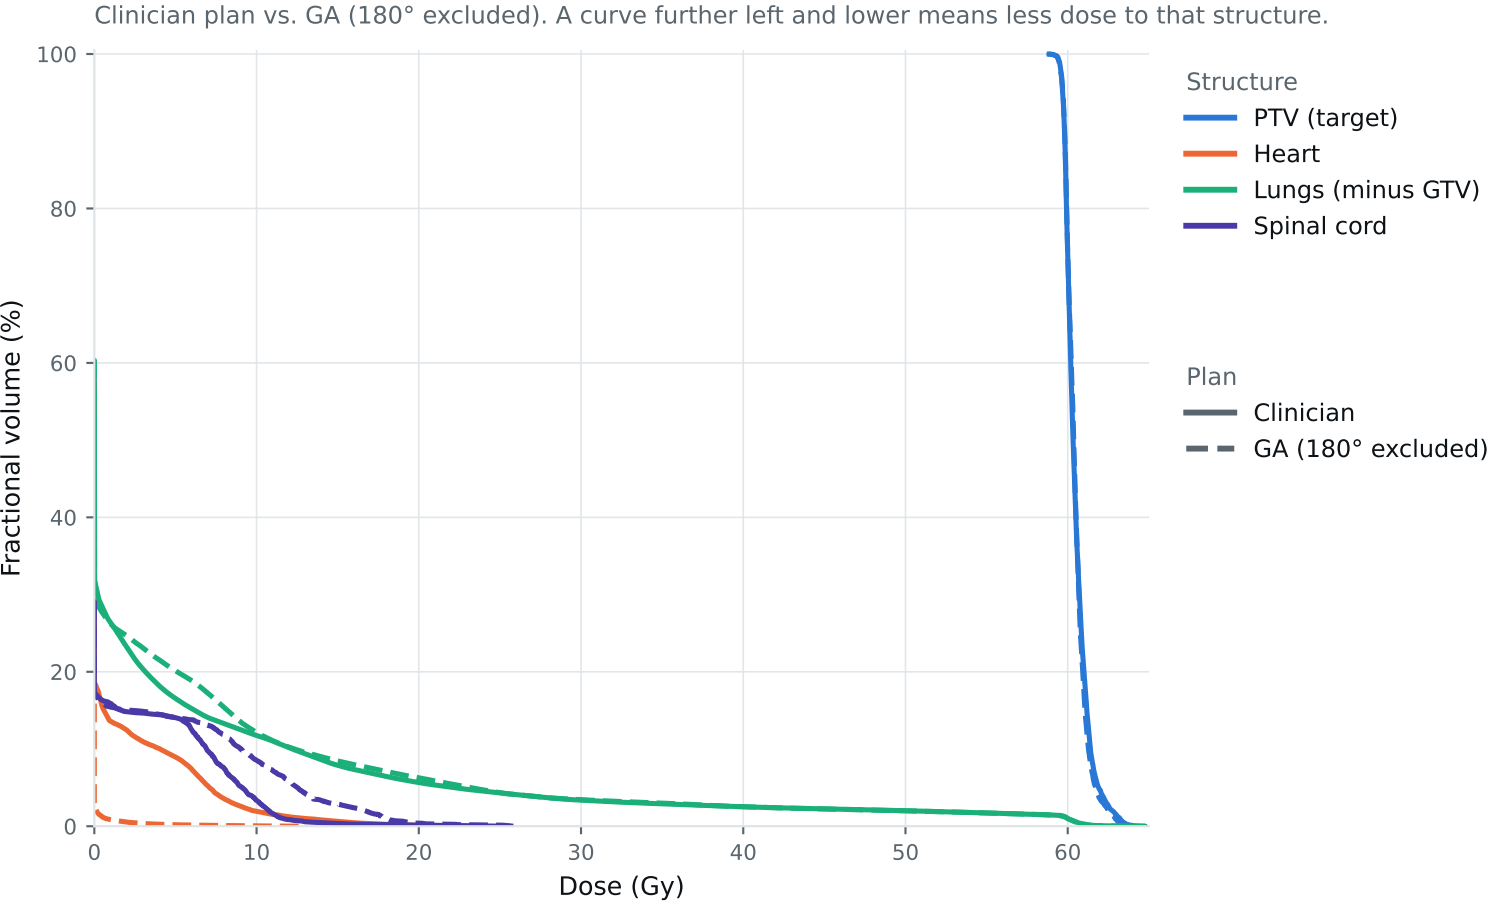

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_32

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

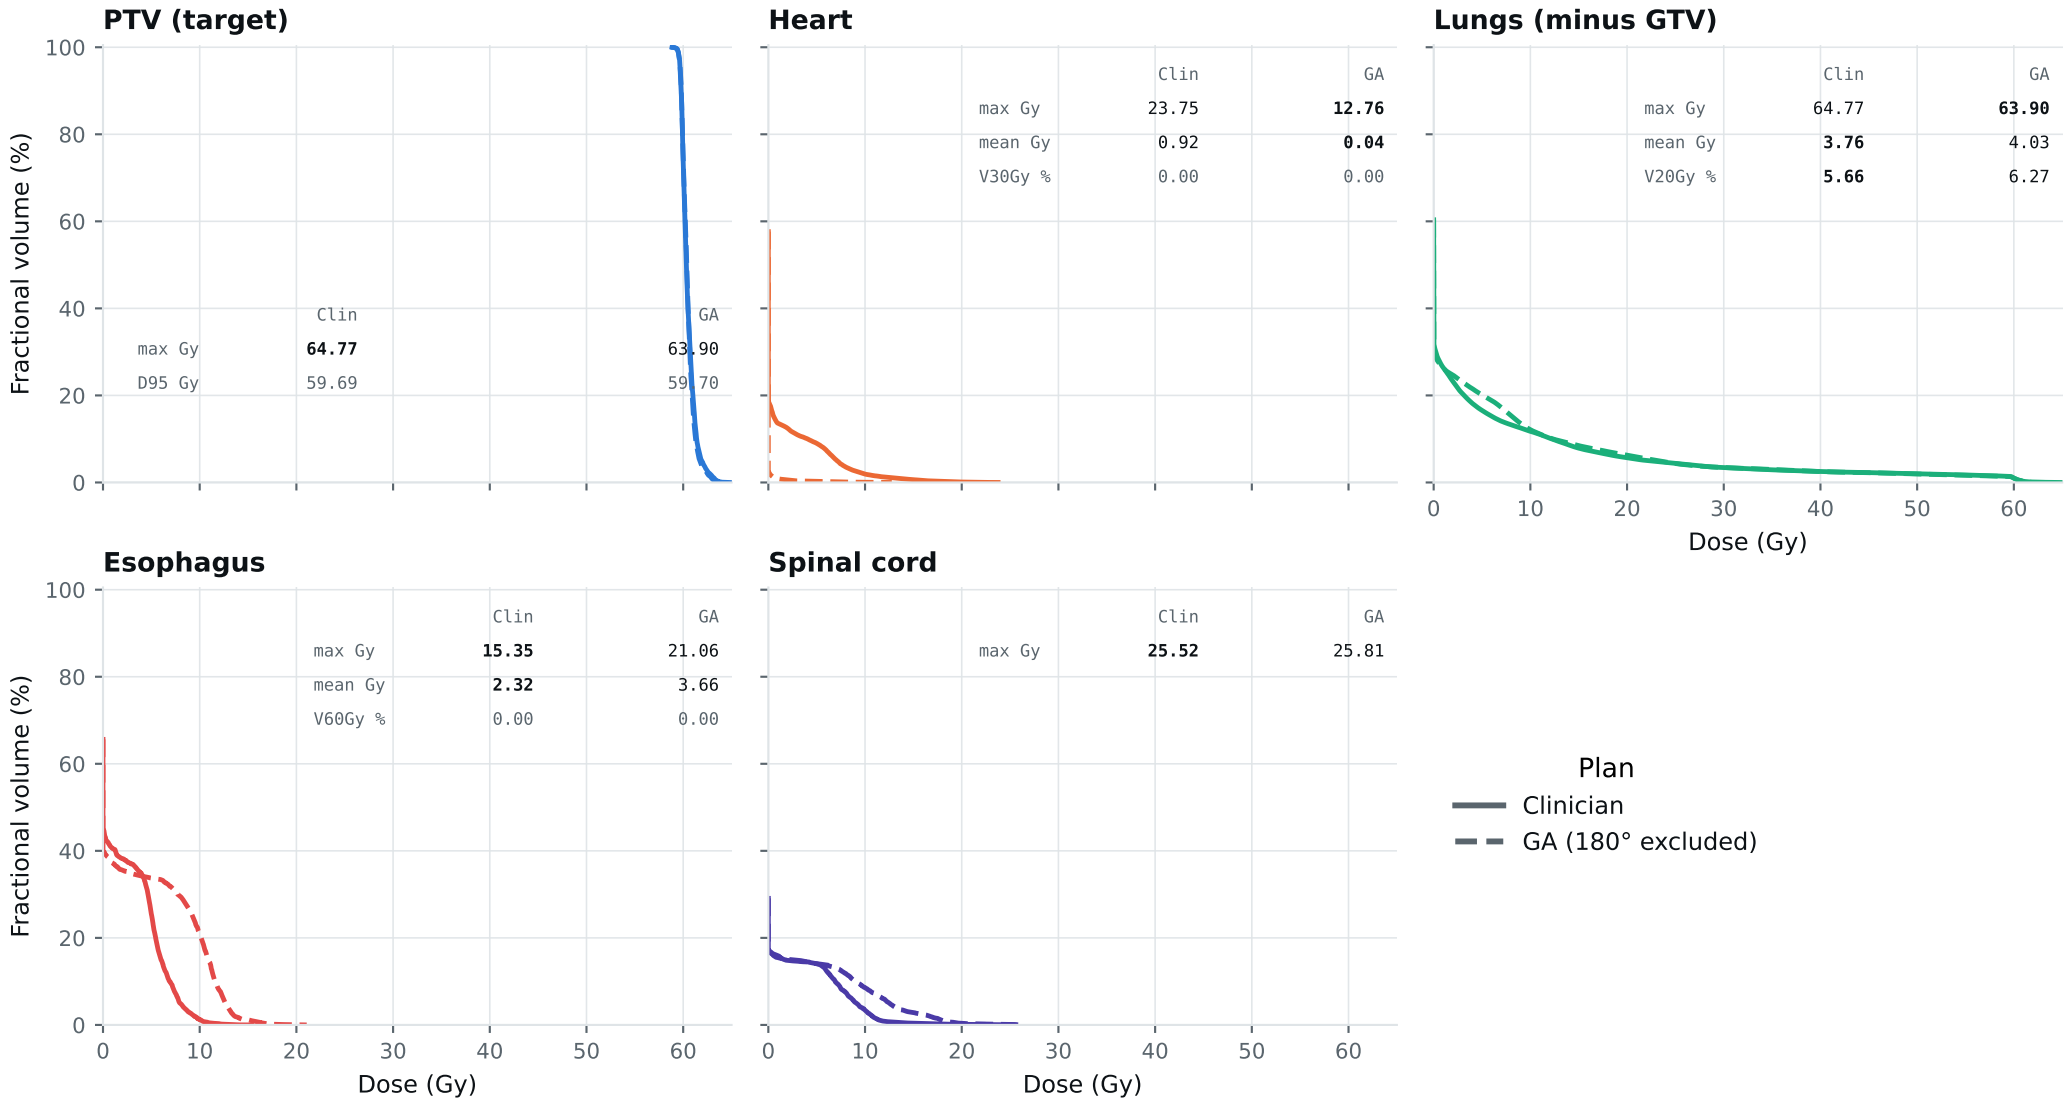

Clinical criteria — Lung_Patient_32

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.48	62.41	Gy
PTV max	69	66	64.77	63.90	Gy
ESOPHAGUS max	66	—	15.35	21.06	Gy
ESOPHAGUS mean	34	21	2.32	3.66	Gy
ESOPHAGUS V60Gy	17	—	0.00	0.00	%
HEART max	66	—	23.75	12.76	Gy
HEART mean	27	20	0.92	0.04	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	11.91	36.09	Gy
LUNG_R max	66	—	64.77	63.90	Gy
CORD max	50	48	25.52	25.81	Gy
SKIN max	60	—	47.68	47.21	Gy
LUNGS_NOT_GTV max	66	—	64.77	63.90	Gy
LUNGS_NOT_GTV mean	21	20	3.76	4.03	Gy
LUNGS_NOT_GTV V20Gy	37	—	5.66	6.27	%
PTV D95 (target coverage)			59.69	59.70	
Objective value (search signal)			45.49	46.13	
MOSEK solve time			12 s	12 s	
Beam angles (gantry°)	Clinician	140°, 355°, 332°, 295°, 240°, 210°, 180°			
	GA	0°, 75°, 90°, 105°, 150°, 195°, 255°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_32_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.