






Dose-volume histogram — Lung_Patient_38

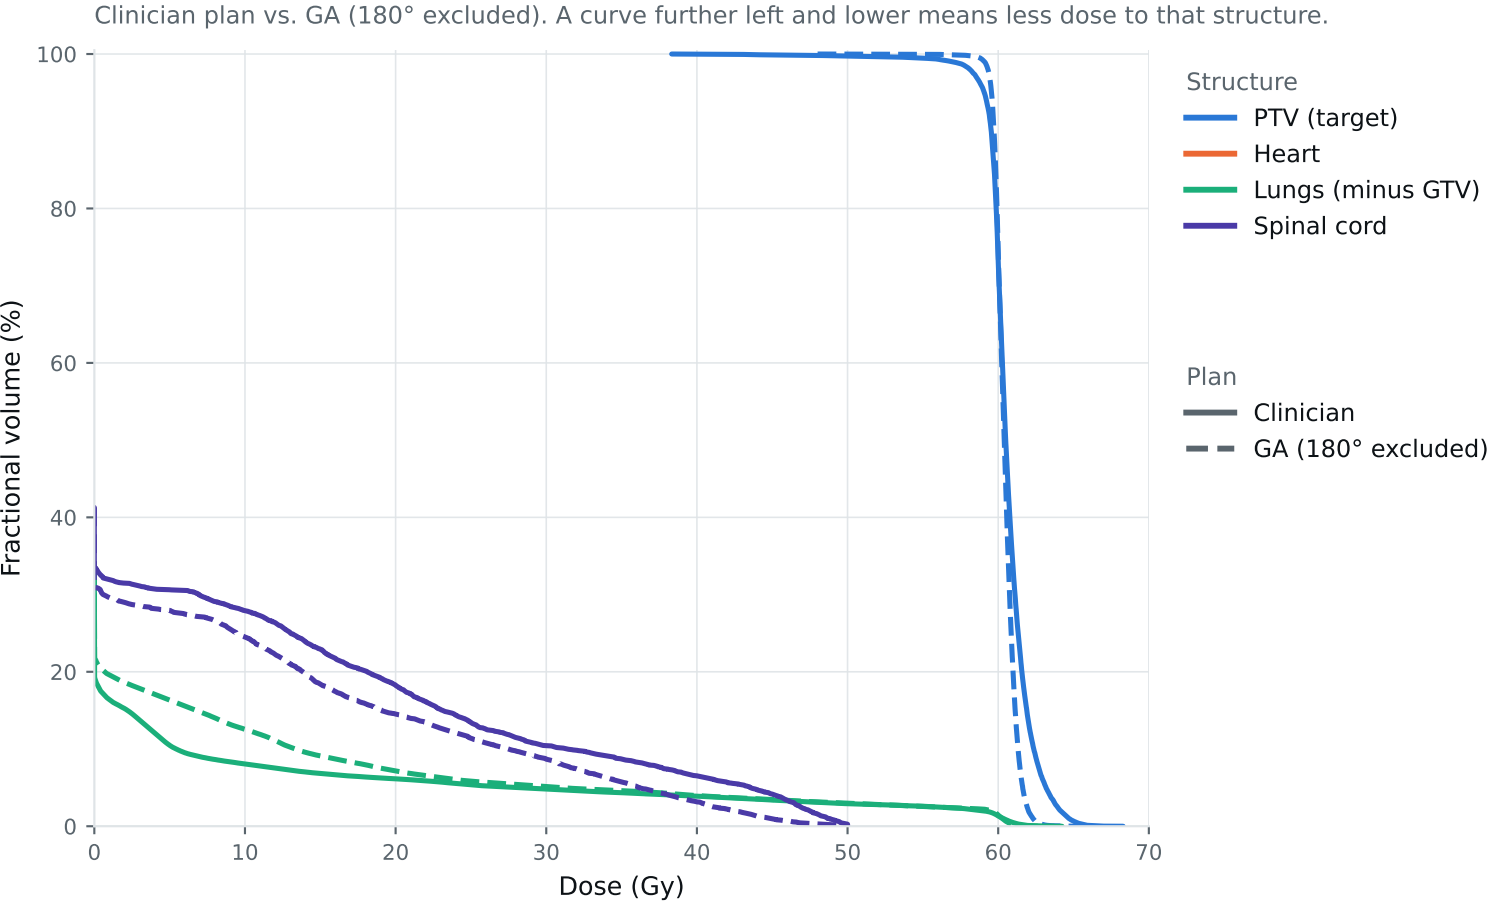

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_38

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal, Grey misses a goal,

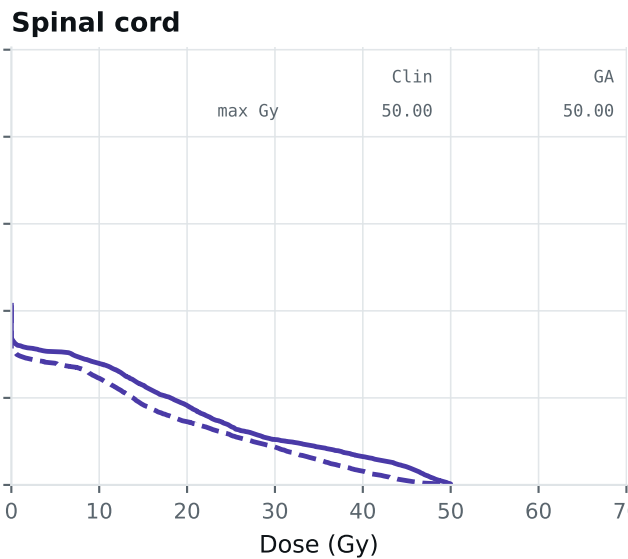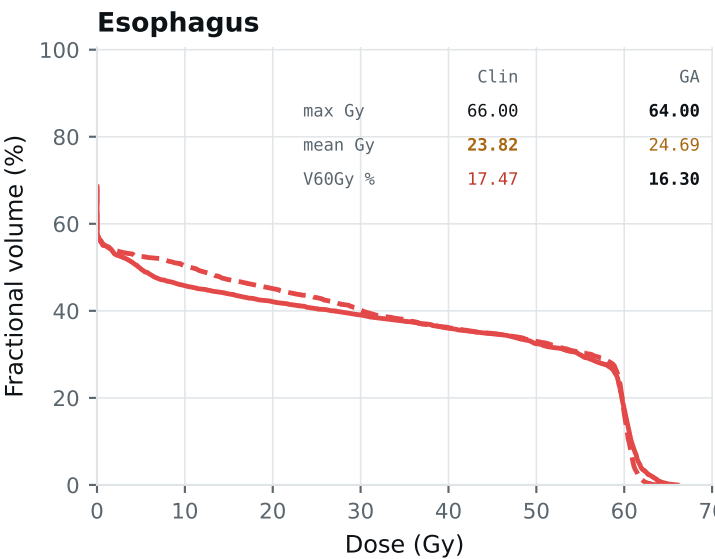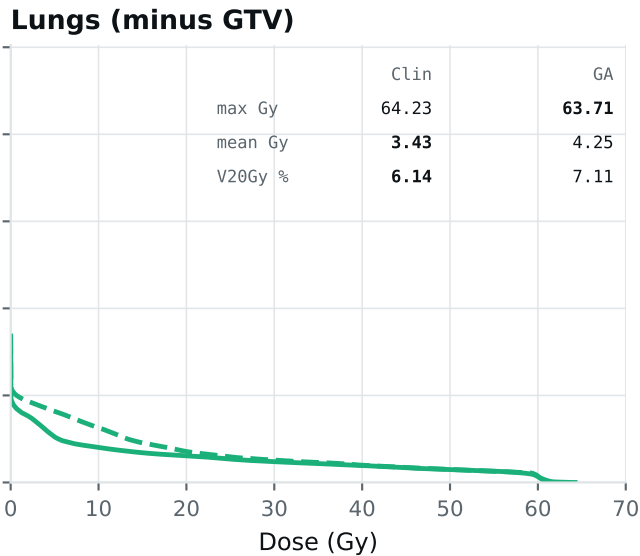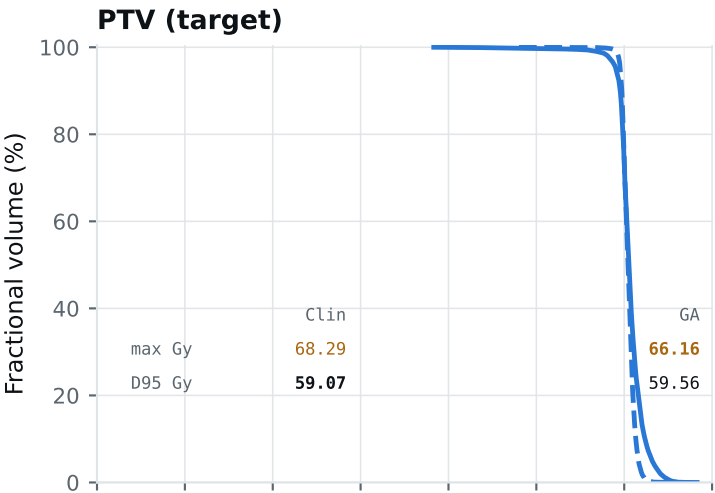

Plan

— Clinician

- - GA (180° excluded)

Clinical criteria — Lung_Patient_38

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	66.82	63.31	Gy
PTV max	69	66	68.29	66.16	Gy
ESOPHAGUS max	66	—	66.00	64.00	Gy
ESOPHAGUS mean	34	21	23.82	24.69	Gy
ESOPHAGUS V60Gy	17	—	17.47	16.30	%
HEART max	66	—	0.00	0.00	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	65.20	63.71	Gy
LUNG_R max	66	—	61.53	60.16	Gy
CORD max	50	48	50.00	50.00	Gy
SKIN max	60	—	60.00	60.00	Gy
LUNGS_NOT_GTV max	66	—	64.23	63.71	Gy
LUNGS_NOT_GTV mean	21	20	3.43	4.25	Gy
LUNGS_NOT_GTV V20Gy	37	—	6.14	7.11	%
PTV D95 (target coverage)			59.07	59.56	
Objective value (search signal)			250.81	119.63	
MOSEK solve time			34 s	37 s	
Beam angles (gantry°)	Clinician	175°, 160°, 140°, 55°, 30°, 0°, 330°			
	GA	160°, 140°, 90°, 195°, 225°, 270°, 345°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_38_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.