



Dose-volume histogram — Lung_Patient_40

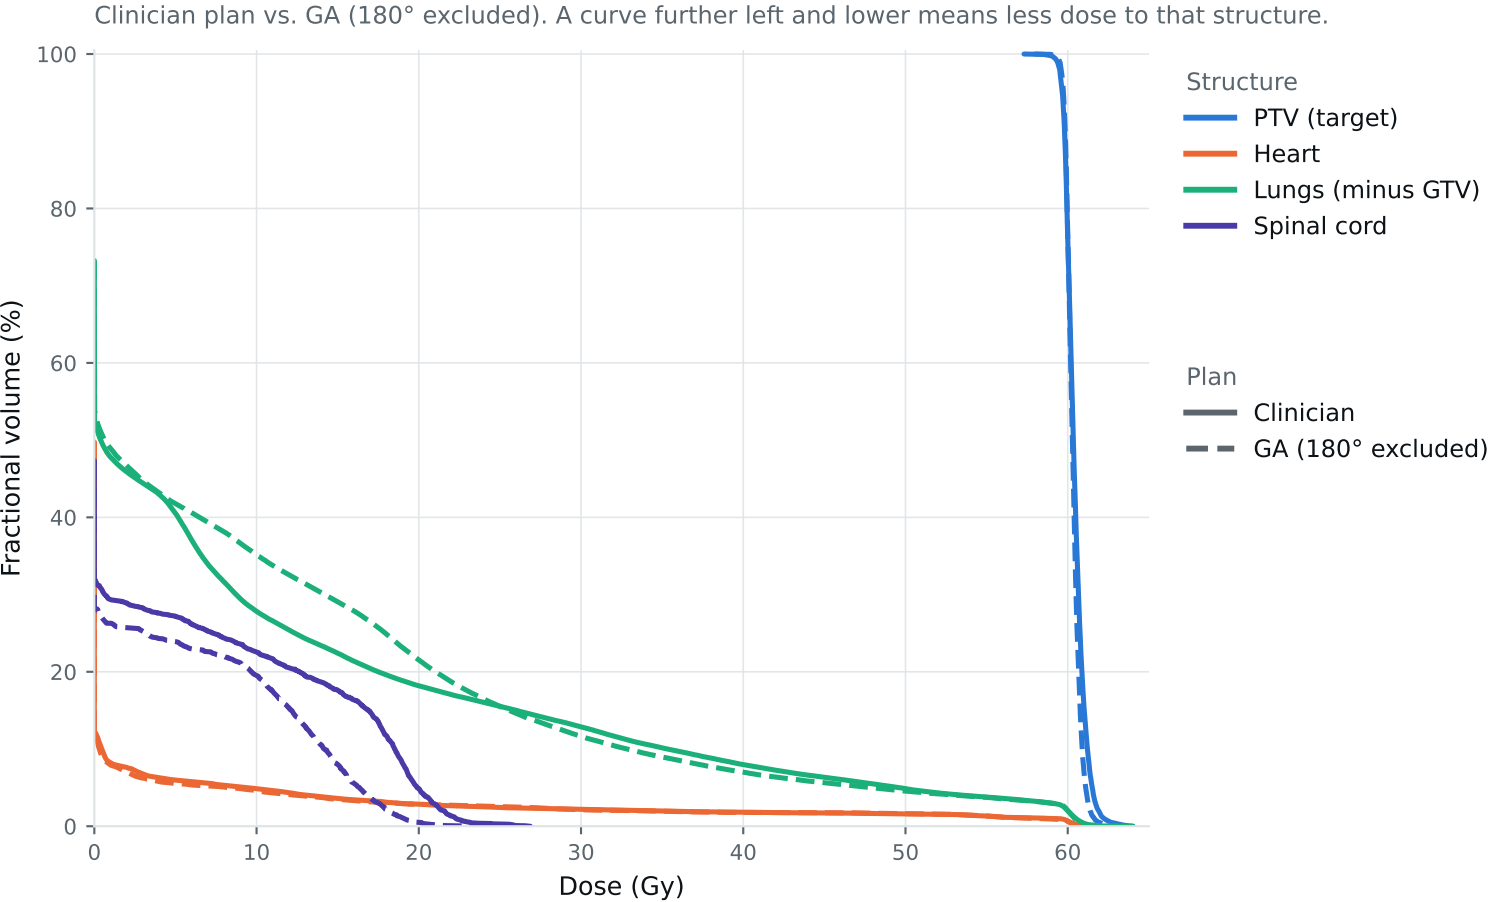

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_40

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

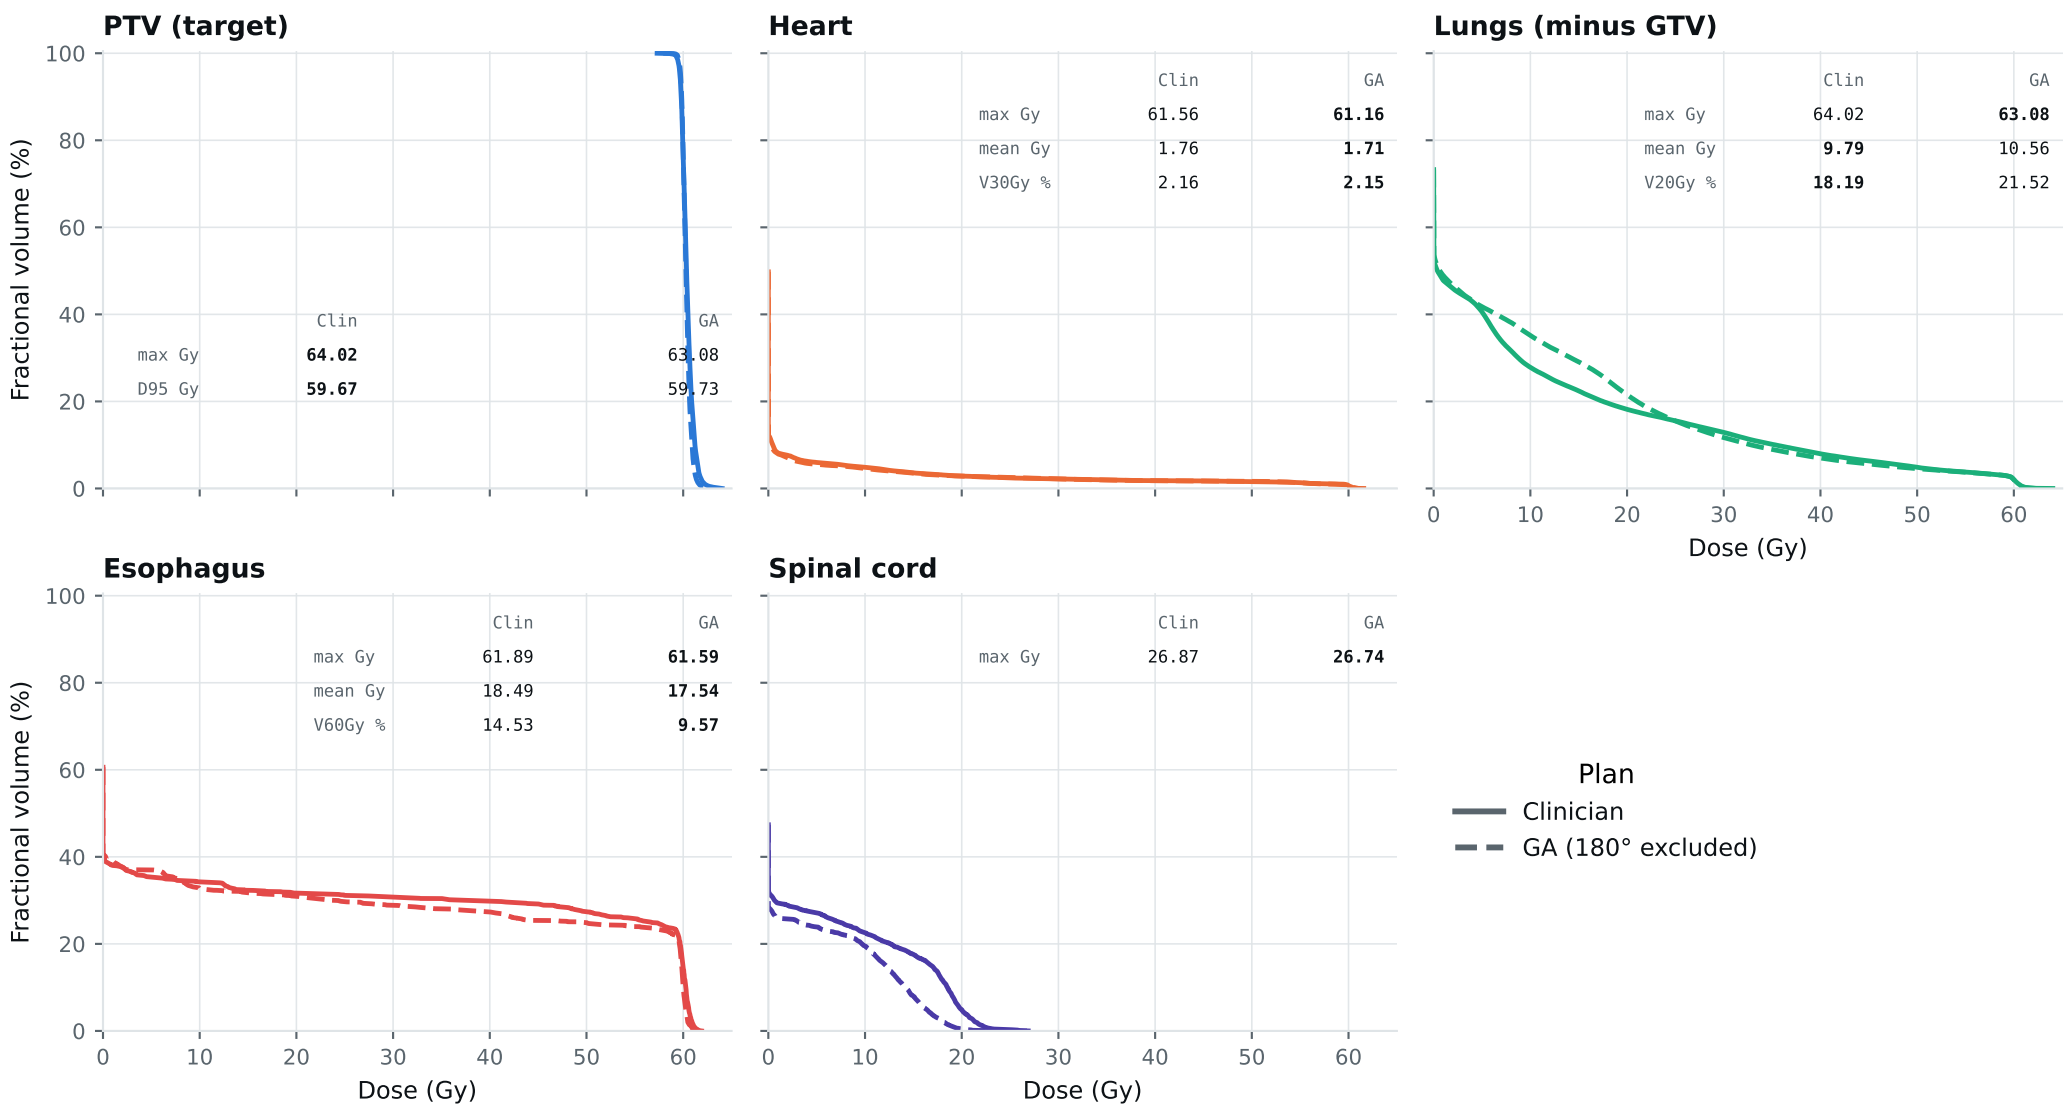

Clinical criteria — Lung_Patient_40

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.70	61.57	Gy
PTV max	69	66	64.02	63.08	Gy
ESOPHAGUS max	66	—	61.89	61.59	Gy
ESOPHAGUS mean	34	21	18.49	17.54	Gy
ESOPHAGUS V60Gy	17	—	14.53	9.57	%
HEART max	66	—	61.56	61.16	Gy
HEART mean	27	20	1.76	1.71	Gy
HEART V30Gy	50	48	2.16	2.15	%
LUNG_L max	66	—	64.02	63.08	Gy
LUNG_R max	66	—	61.52	61.65	Gy
CORD max	50	48	26.87	26.74	Gy
SKIN max	60	—	48.57	48.34	Gy
LUNGS_NOT_GTV max	66	—	64.02	63.08	Gy
LUNGS_NOT_GTV mean	21	20	9.79	10.56	Gy
LUNGS_NOT_GTV V20Gy	37	—	18.19	21.52	%
PTV D95 (target coverage)			59.67	59.73	
Objective value (search signal)			97.53	89.85	
MOSEK solve time			28 s	27 s	
Beam angles (gantry°)	Clinician	175°, 155°, 120°, 55°, 25°, 0°			
	GA	0°, 75°, 135°, 165°, 195°, 255°, 285°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_40_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.