





Dose-volume histogram — Lung_Patient_23

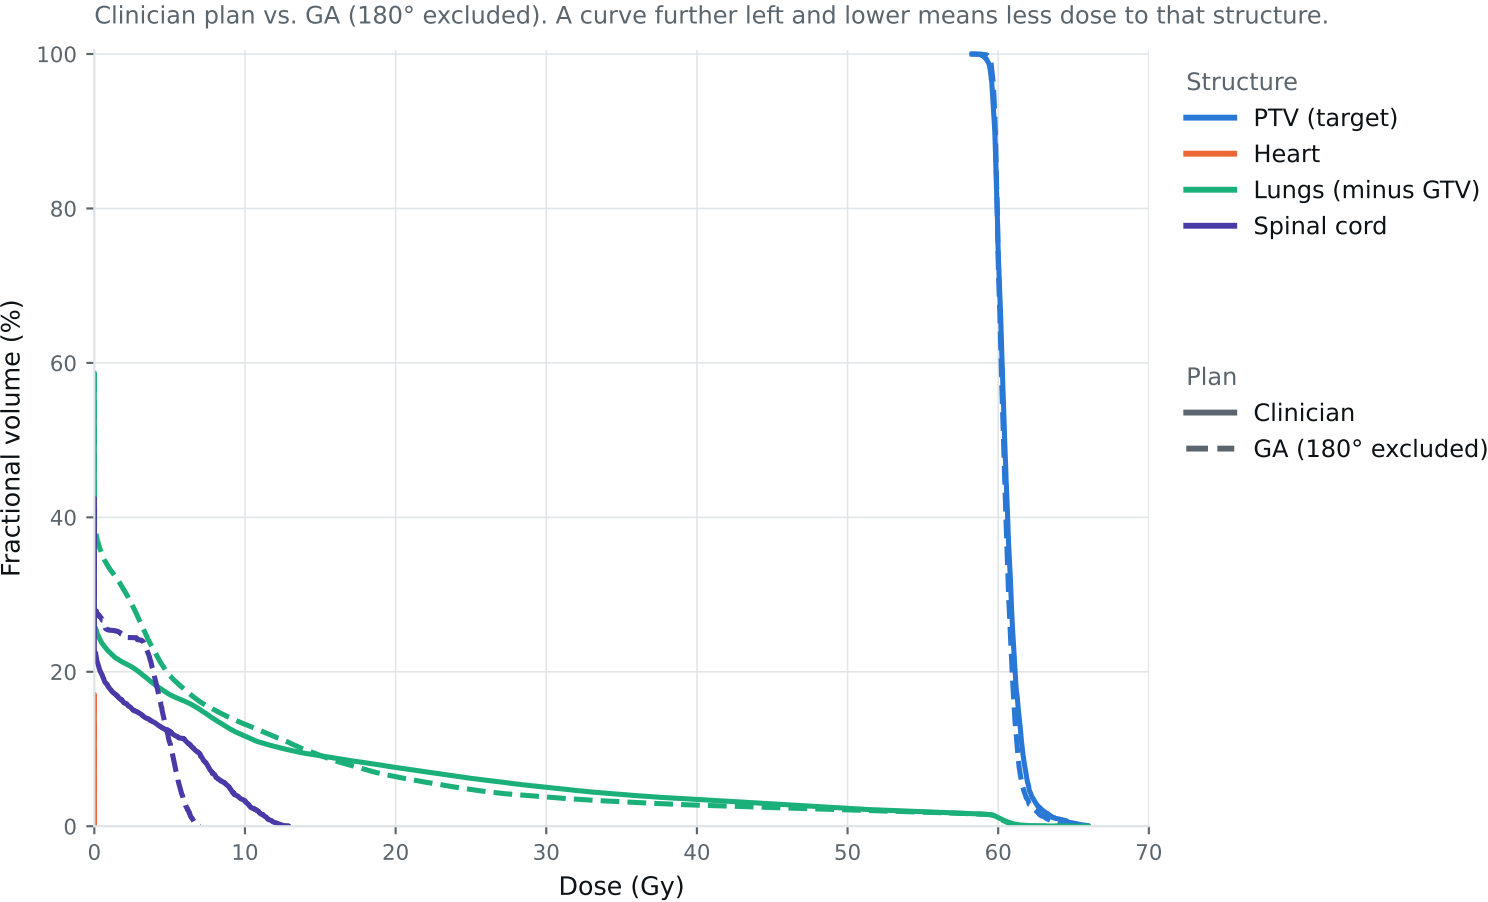

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_23

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

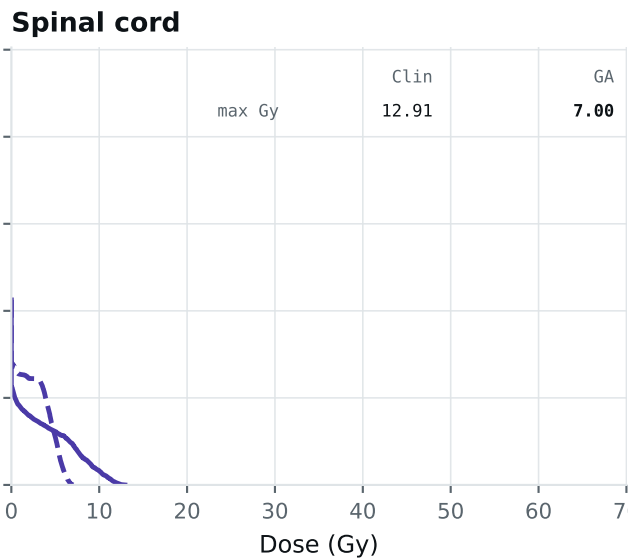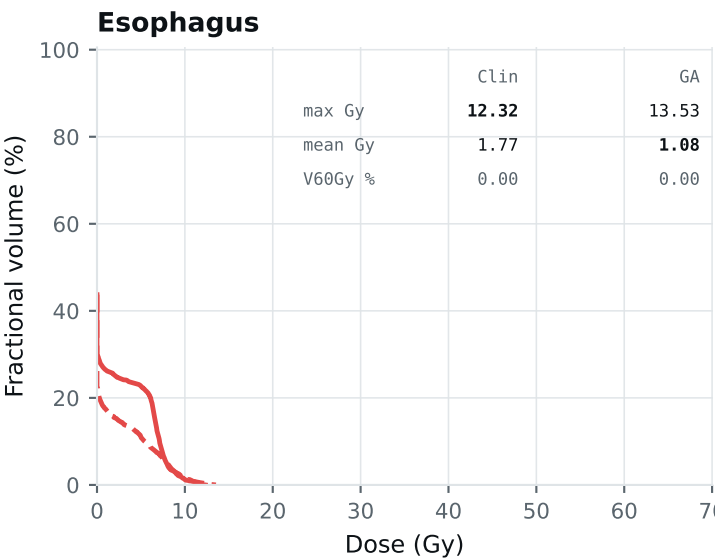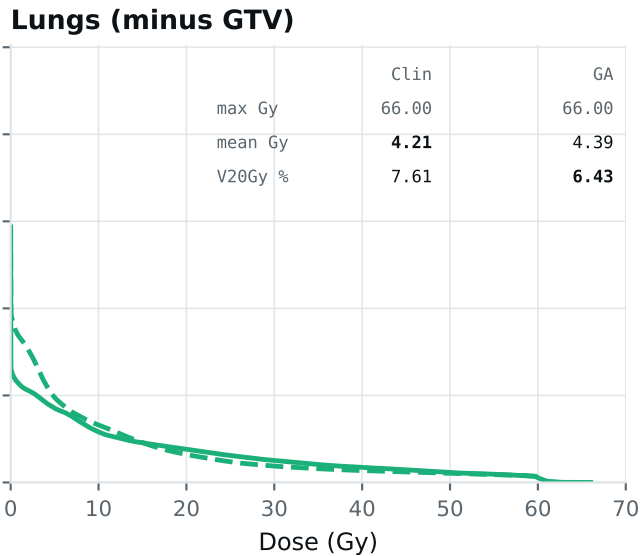

Plan

- Clinician
- - GA (180° excluded)

Clinical criteria — Lung_Patient_23

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	63.54	64.05	Gy
PTV max	69	66	66.00	66.00	Gy
ESOPHAGUS max	66	—	12.32	13.53	Gy
ESOPHAGUS mean	34	21	1.77	1.08	Gy
ESOPHAGUS V60Gy	17	—	0.00	0.00	%
HEART max	66	—	0.00	0.00	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	66.00	66.00	Gy
LUNG_R max	66	—	13.81	21.97	Gy
CORD max	50	48	12.91	7.00	Gy
SKIN max	60	—	42.49	40.91	Gy
LUNGS_NOT_GTV max	66	—	66.00	66.00	Gy
LUNGS_NOT_GTV mean	21	20	4.21	4.39	Gy
LUNGS_NOT_GTV V20Gy	37	—	7.61	6.43	%
PTV D95 (target coverage)			59.63	59.71	
Objective value (search signal)			52.79	44.30	
MOSEK solve time			10 s	11 s	
Beam angles (gantry°)	Clinician	175°, 145°, 120°, 55°, 25°, 0°, 340°			
	GA	0°, 45°, 75°, 90°, 105°, 195°, 330°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_23_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.