



Dose-volume histogram — Lung_Patient_29

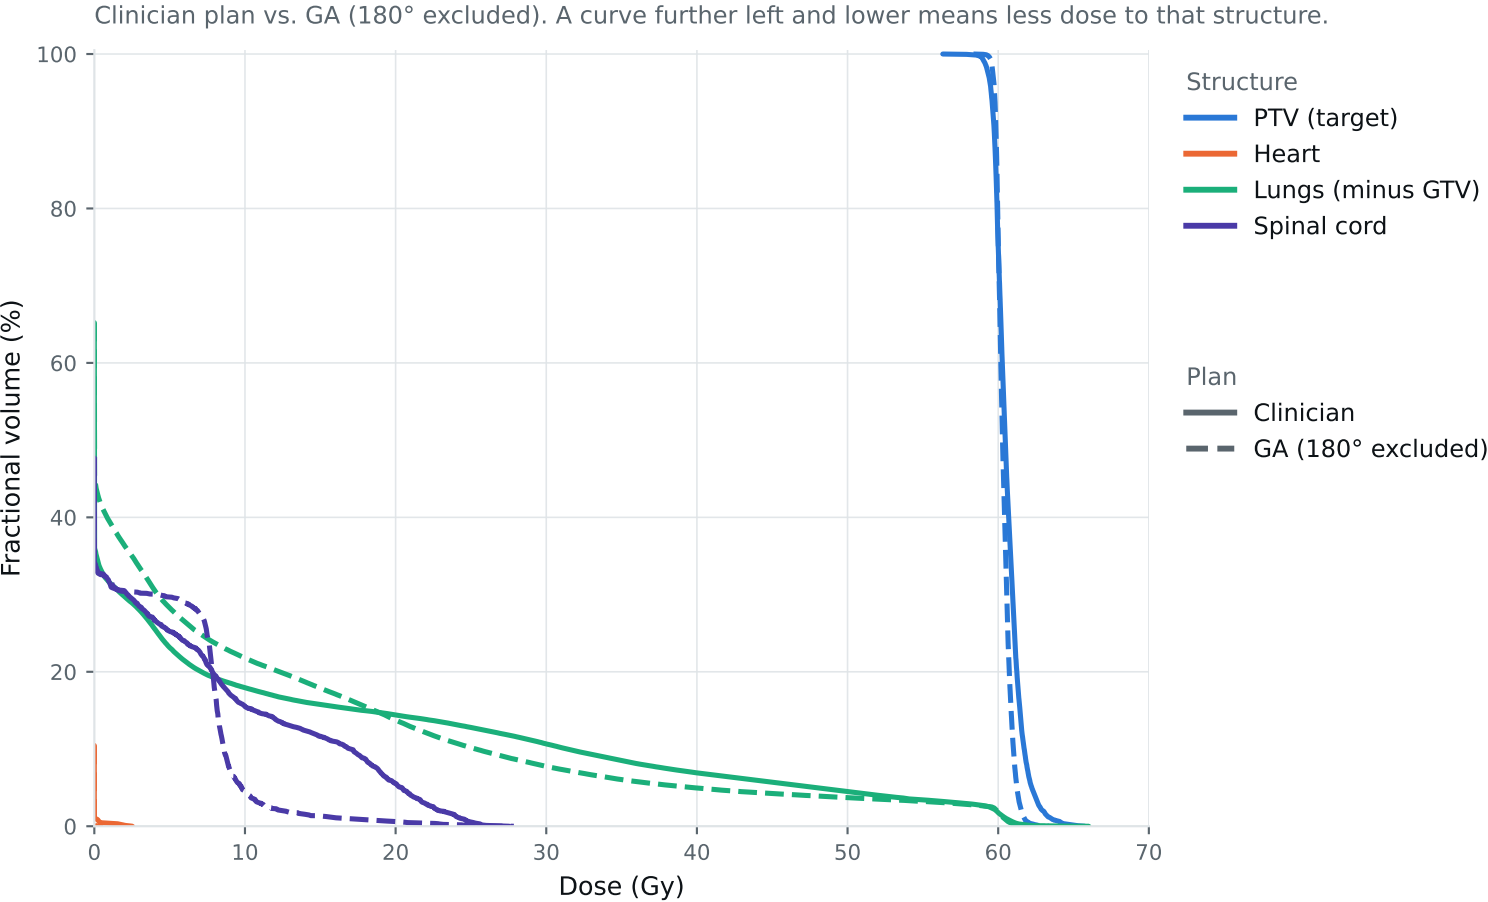

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_29

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

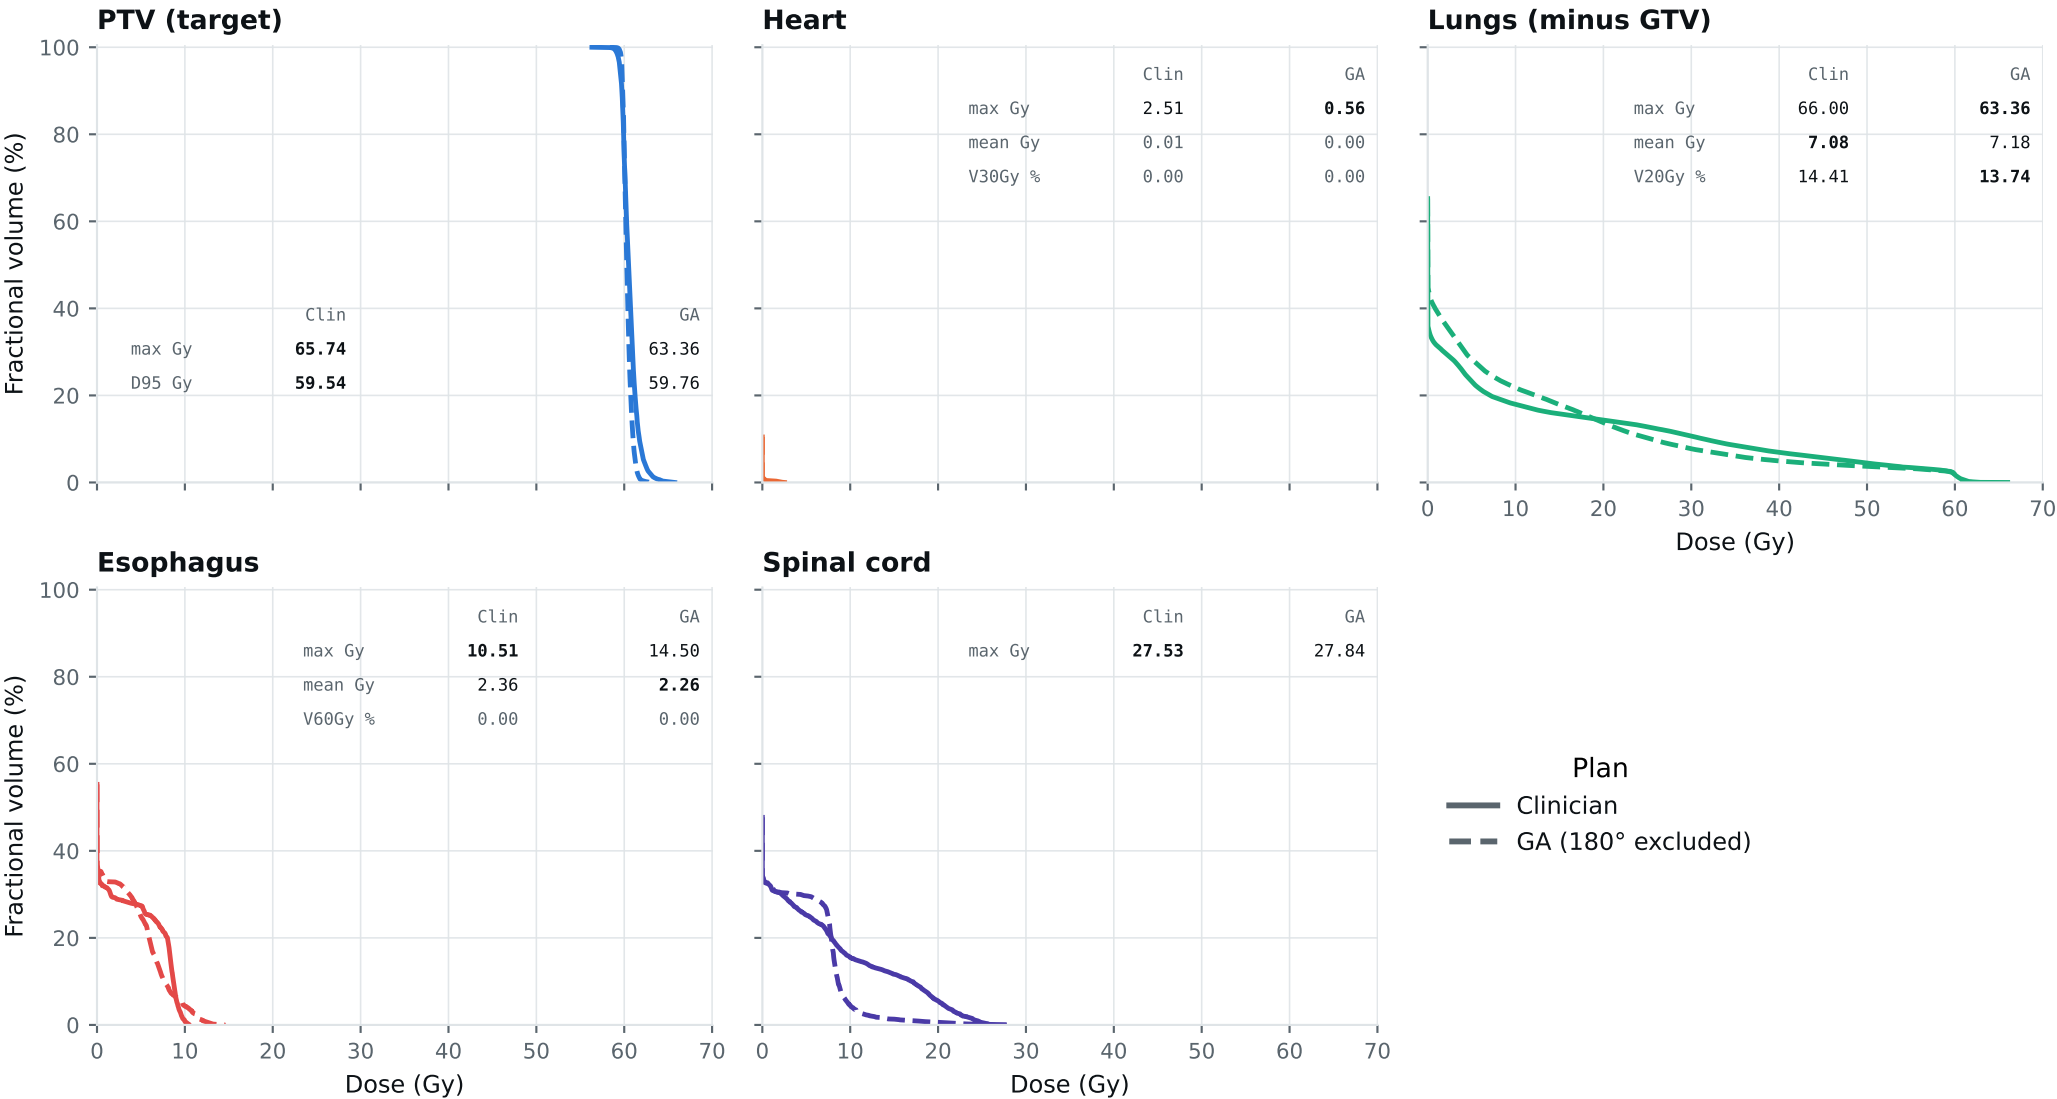

Clinical criteria — Lung_Patient_29

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	64.96	62.13	Gy
PTV max	69	66	65.74	63.36	Gy
ESOPHAGUS max	66	—	10.51	14.50	Gy
ESOPHAGUS mean	34	21	2.36	2.26	Gy
ESOPHAGUS V60Gy	17	—	0.00	0.00	%
HEART max	66	—	2.51	0.56	Gy
HEART mean	27	20	0.01	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	16.48	37.70	Gy
LUNG_R max	66	—	66.00	63.36	Gy
CORD max	50	48	27.53	27.84	Gy
SKIN max	60	—	43.85	44.98	Gy
LUNGS_NOT_GTV max	66	—	66.00	63.36	Gy
LUNGS_NOT_GTV mean	21	20	7.08	7.18	Gy
LUNGS_NOT_GTV V20Gy	37	—	14.41	13.74	%
PTV D95 (target coverage)			59.54	59.76	
Objective value (search signal)			65.81	47.40	
MOSEK solve time			22 s	23 s	
Beam angles (gantry°)	Clinician	165°, 0°, 330°, 300°, 235°, 210°, 185°			
	GA	165°, 30°, 75°, 195°, 270°, 285°, 315°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_29_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.