



Dose-volume histogram — Lung_Patient_30

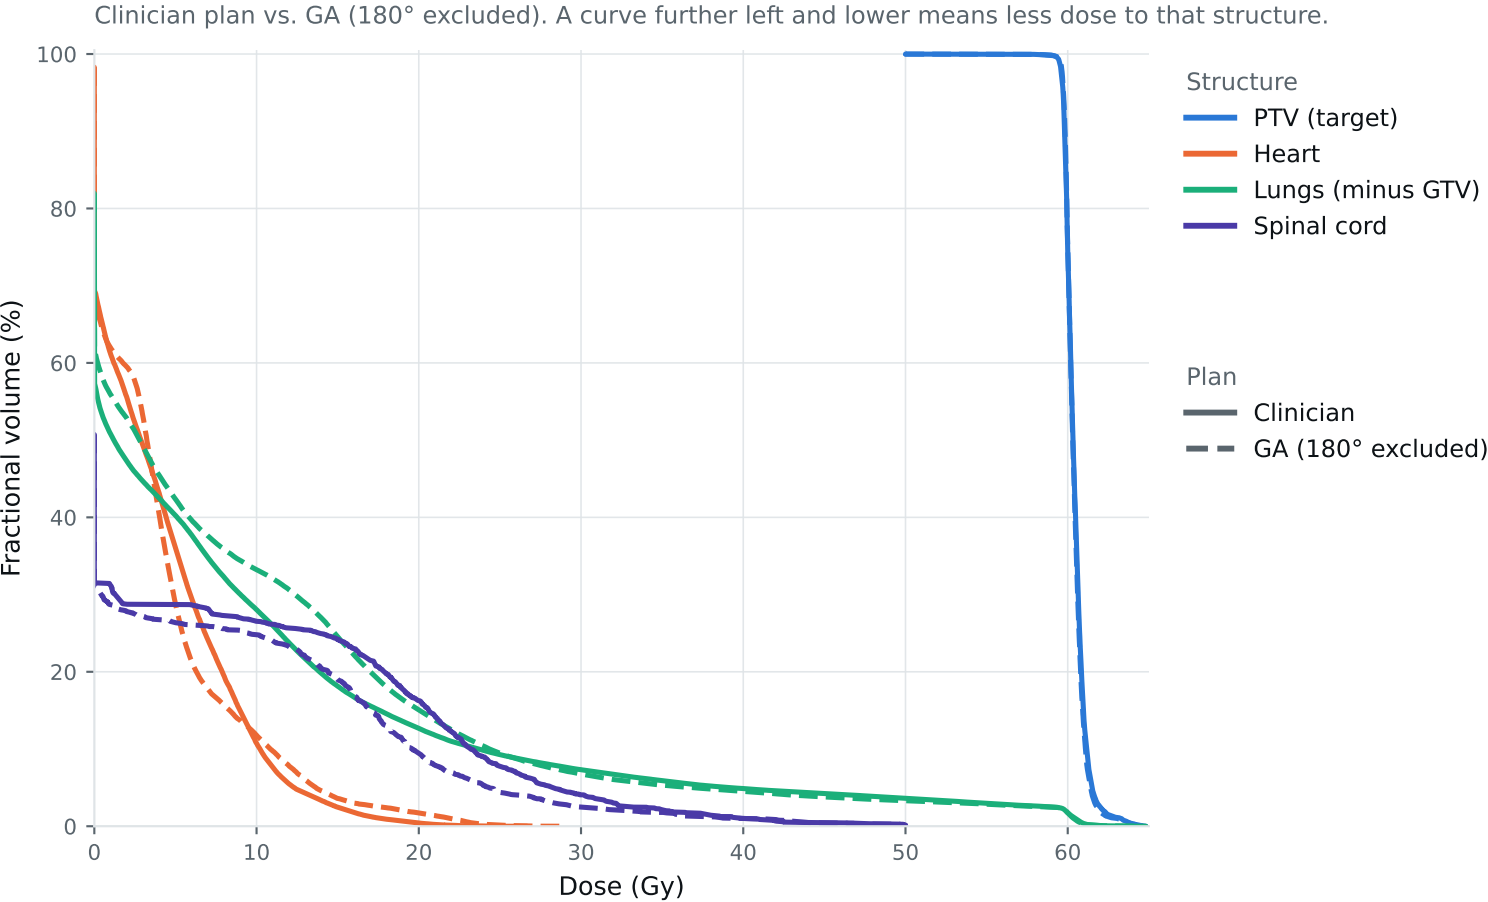

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_30

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

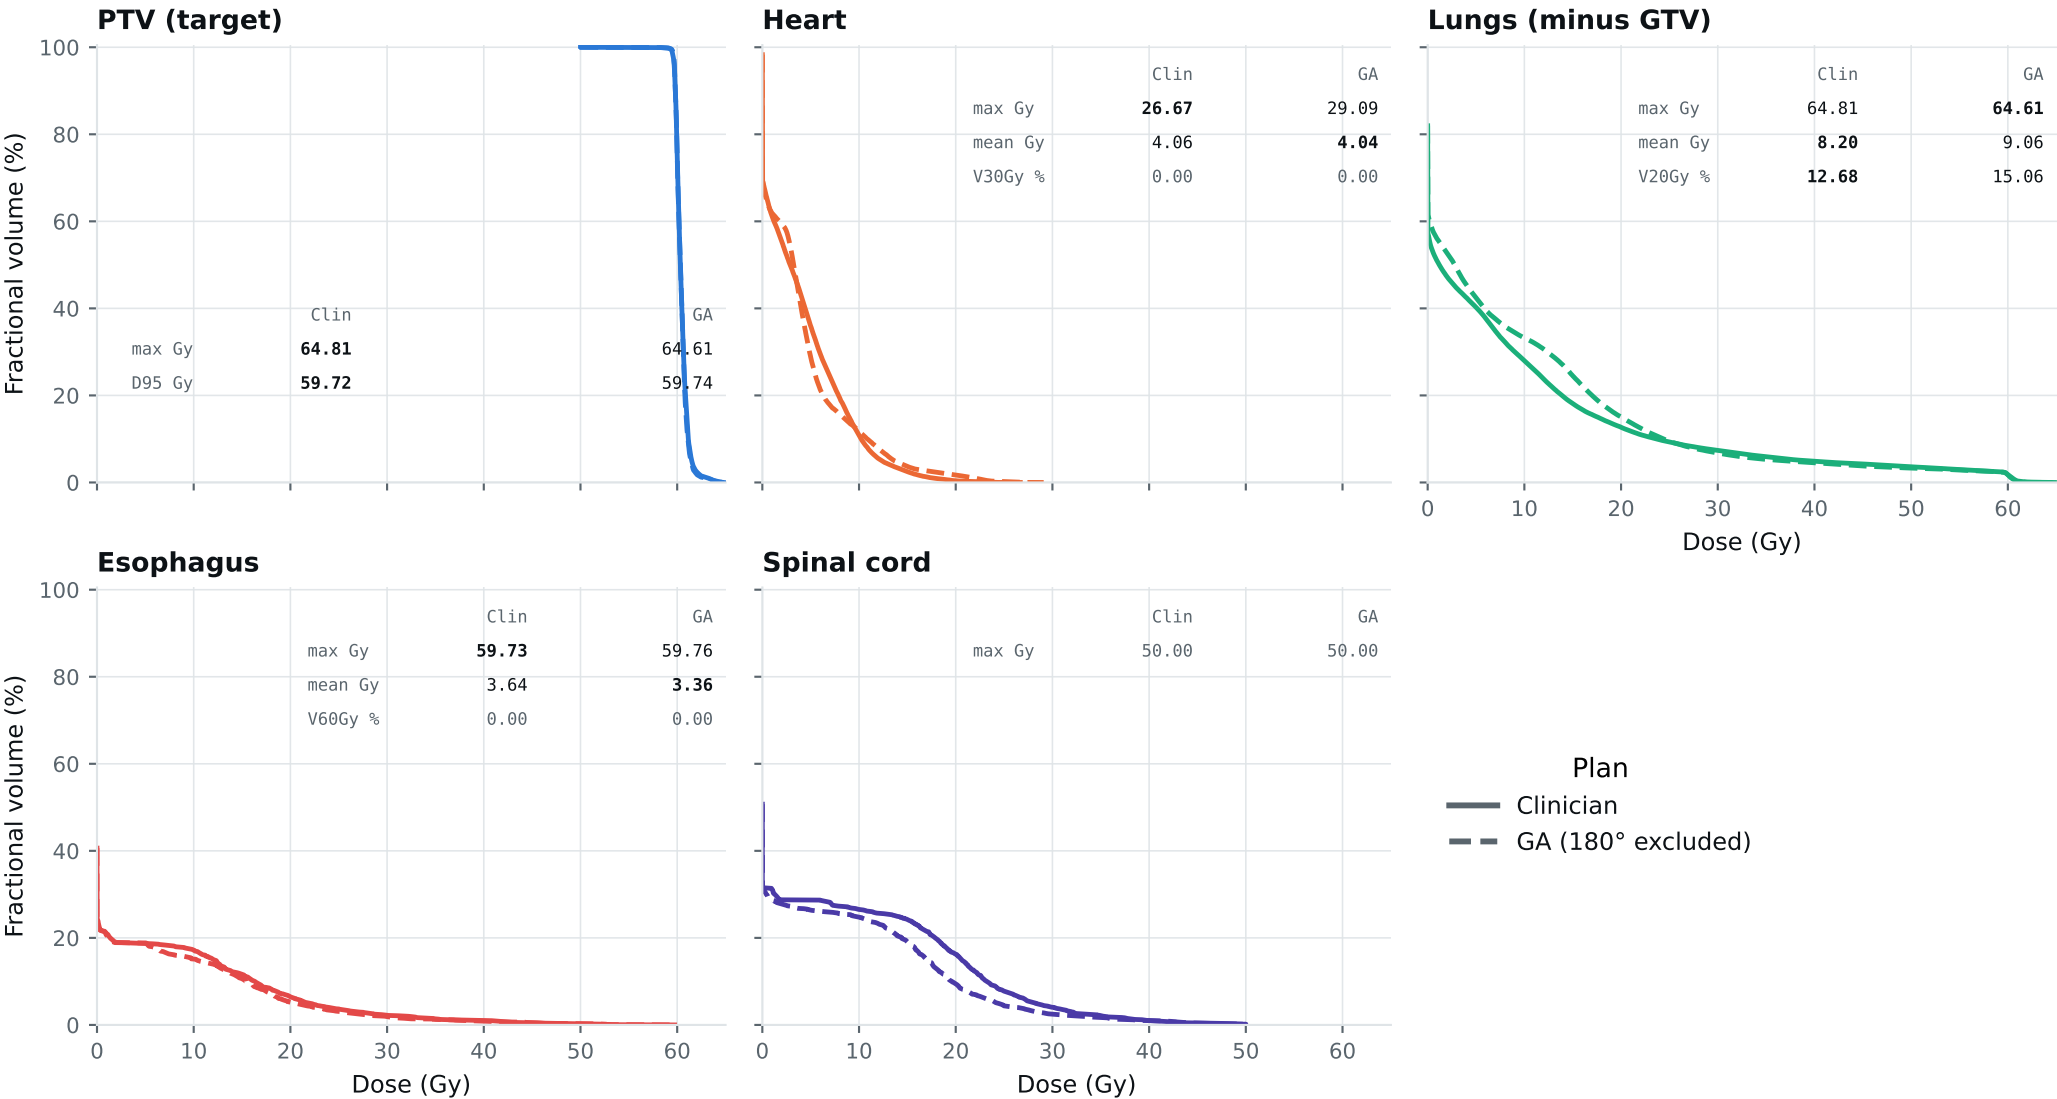

Clinical criteria — Lung_Patient_30

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	61.83	61.57	Gy
PTV max	69	66	64.81	64.61	Gy
ESOPHAGUS max	66	—	59.73	59.76	Gy
ESOPHAGUS mean	34	21	3.64	3.36	Gy
ESOPHAGUS V60Gy	17	—	0.00	0.00	%
HEART max	66	—	26.67	29.09	Gy
HEART mean	27	20	4.06	4.04	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	33.95	39.57	Gy
LUNG_R max	66	—	64.81	64.61	Gy
CORD max	50	48	50.00	50.00	Gy
SKIN max	60	—	44.46	44.36	Gy
LUNGS_NOT_GTV max	66	—	64.81	64.61	Gy
LUNGS_NOT_GTV mean	21	20	8.20	9.06	Gy
LUNGS_NOT_GTV V20Gy	37	—	12.68	15.06	%
PTV D95 (target coverage)			59.72	59.74	
Objective value (search signal)			64.30	61.27	
MOSEK solve time			14 s	17 s	
Beam angles (gantry°)	Clinician	140°, 340°, 300°, 240°, 210°, 180°			
	GA	140°, 0°, 75°, 105°, 195°, 225°, 345°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_30_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.