






Dose-volume histogram — Lung_Patient_16

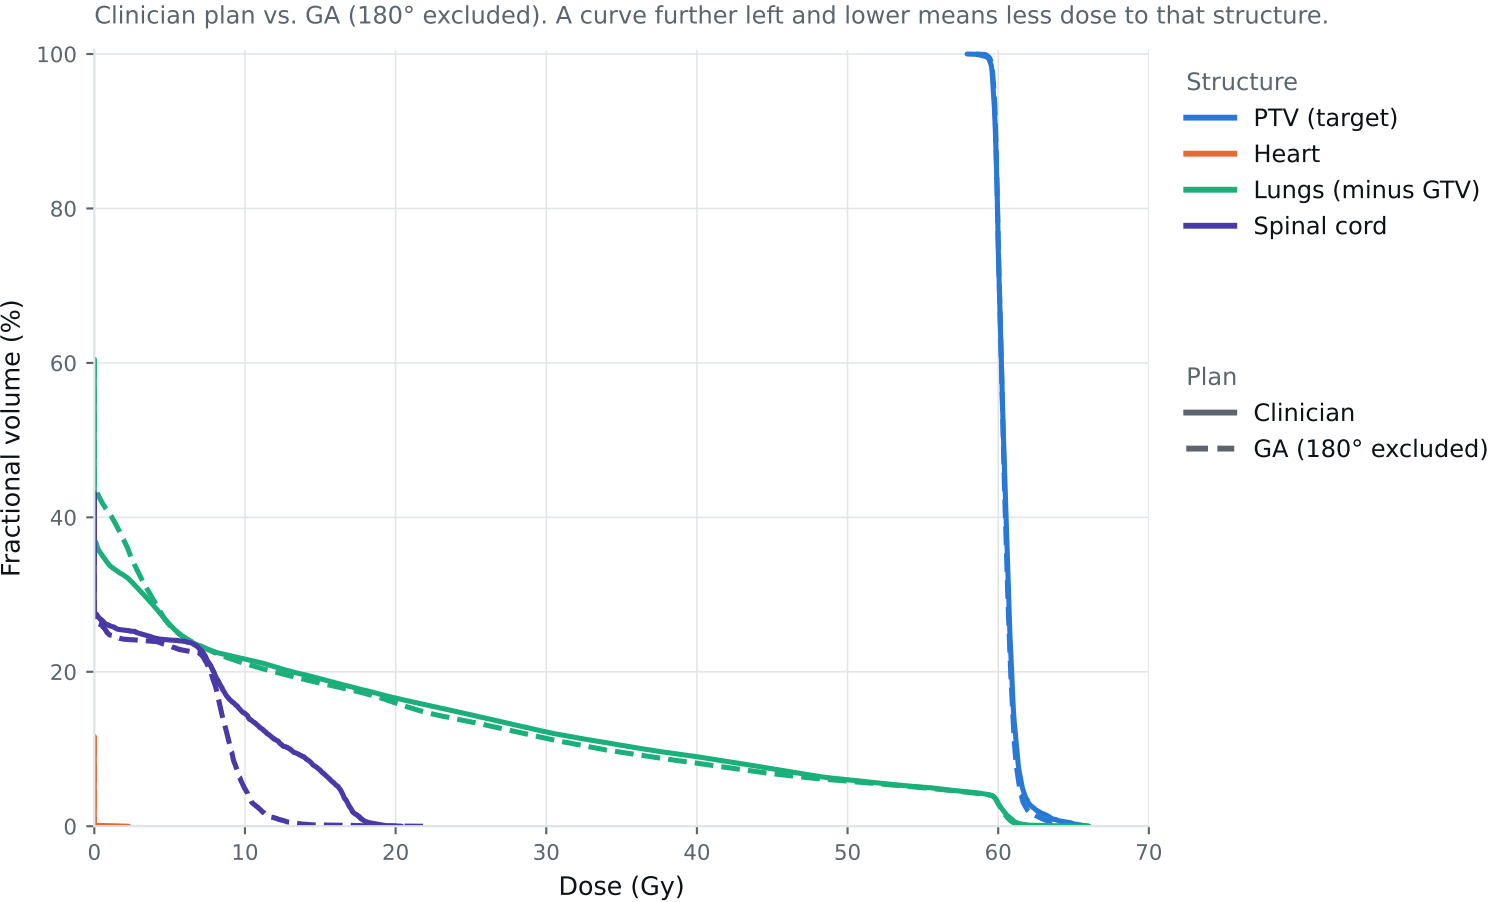

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_16

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

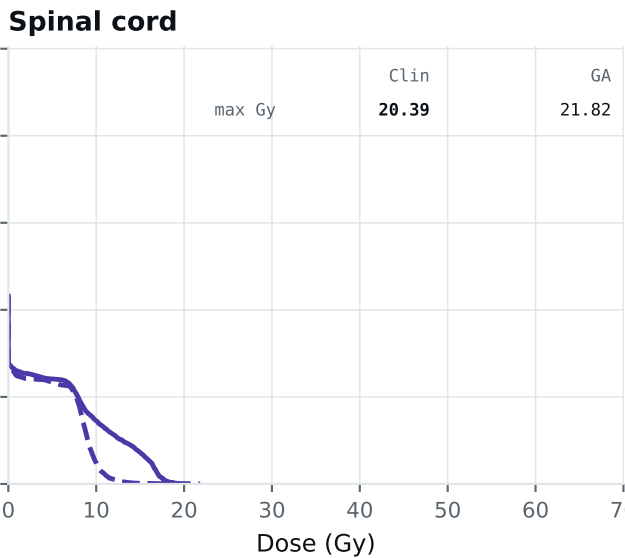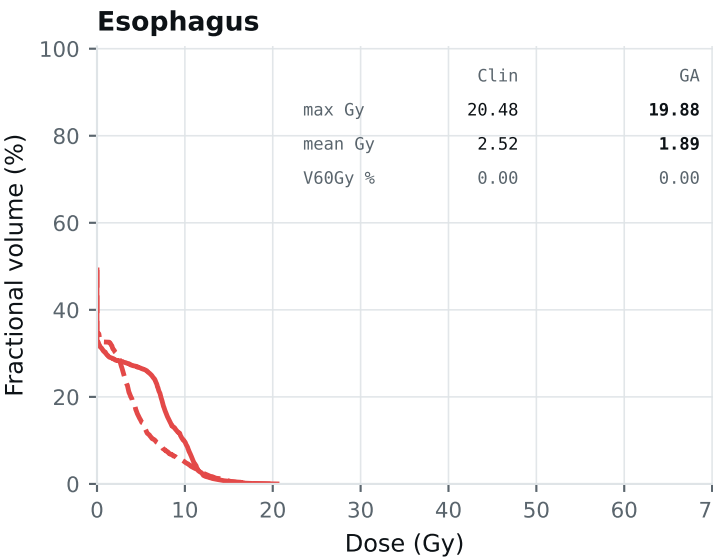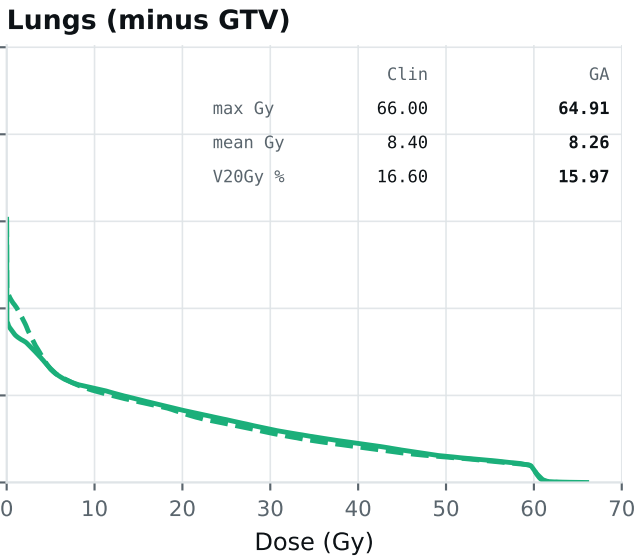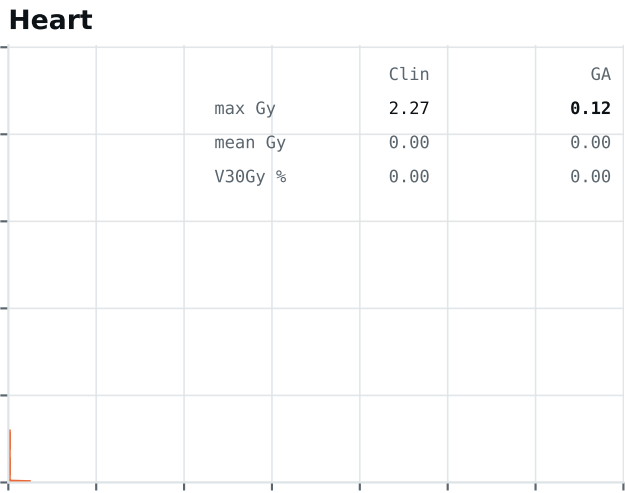

Plan
— Clinician
- - GA (180° excluded)

Clinical criteria — Lung_Patient_16

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.11	62.05	Gy
PTV max	69	66	66.00	64.91	Gy
ESOPHAGUS max	66	—	20.48	19.88	Gy
ESOPHAGUS mean	34	21	2.52	1.89	Gy
ESOPHAGUS V60Gy	17	—	0.00	0.00	%
HEART max	66	—	2.27	0.12	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	9.53	34.55	Gy
LUNG_R max	66	—	66.00	64.91	Gy
CORD max	50	48	20.39	21.82	Gy
SKIN max	60	—	38.93	40.82	Gy
LUNGS_NOT_GTV max	66	—	66.00	64.91	Gy
LUNGS_NOT_GTV mean	21	20	8.40	8.26	Gy
LUNGS_NOT_GTV V20Gy	37	—	16.60	15.97	%
PTV D95 (target coverage)			59.70	59.73	
Objective value (search signal)			59.58	53.13	
Solve time			17 s	18 s	
Beam angles (gantry°)	Clinician	0°, 334°, 310°, 245°, 212°, 185°			
	GA	185°, 30°, 225°, 255°, 270°, 300°, 345°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_16_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.