



Dose-volume histogram — Lung_Patient_11

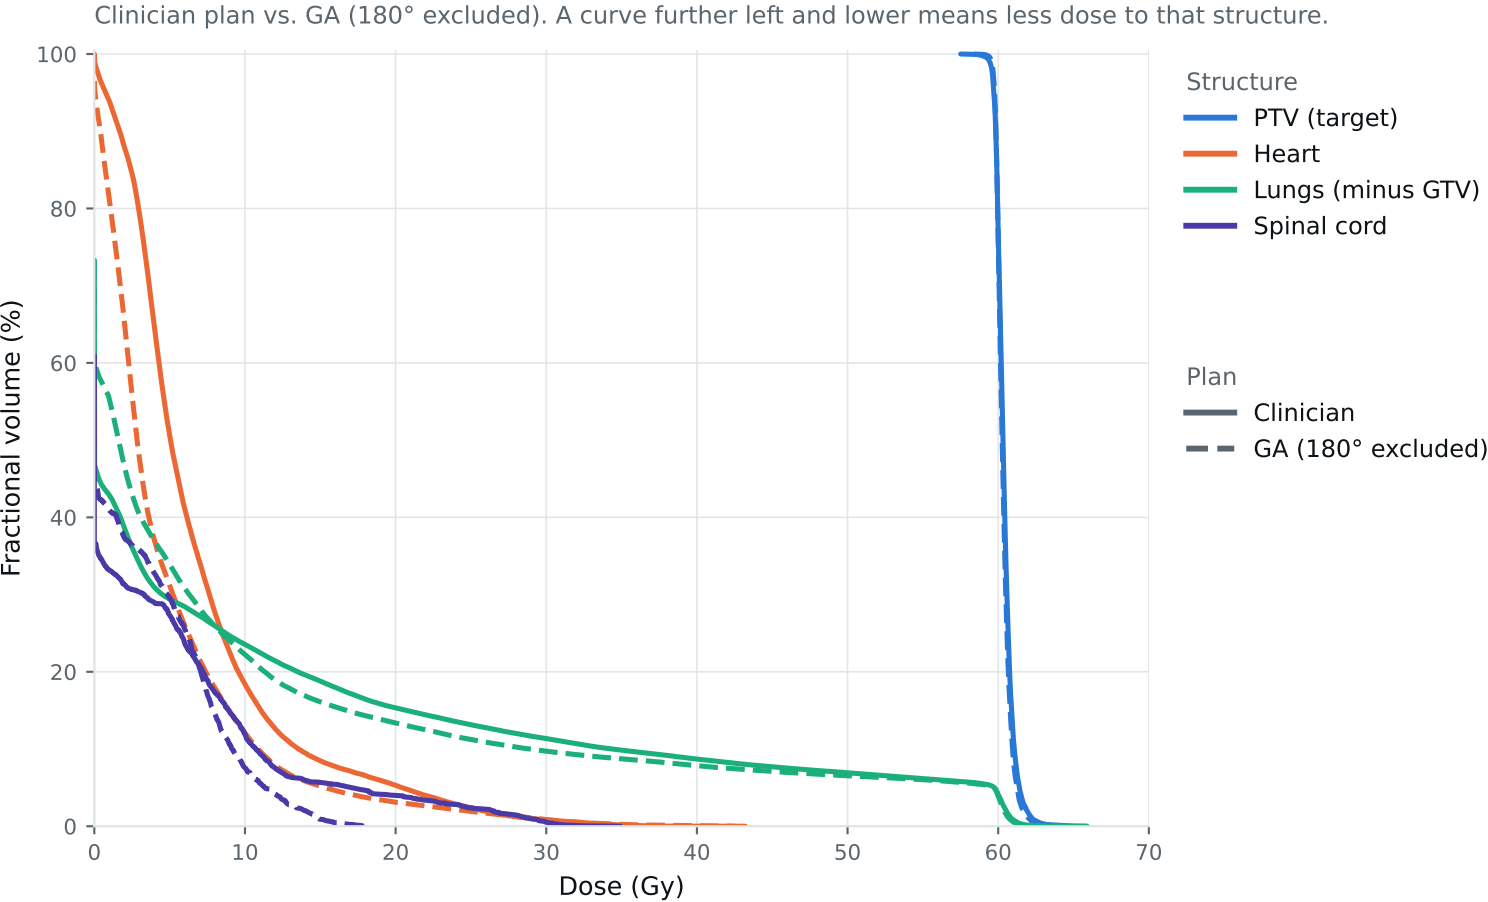

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_11

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

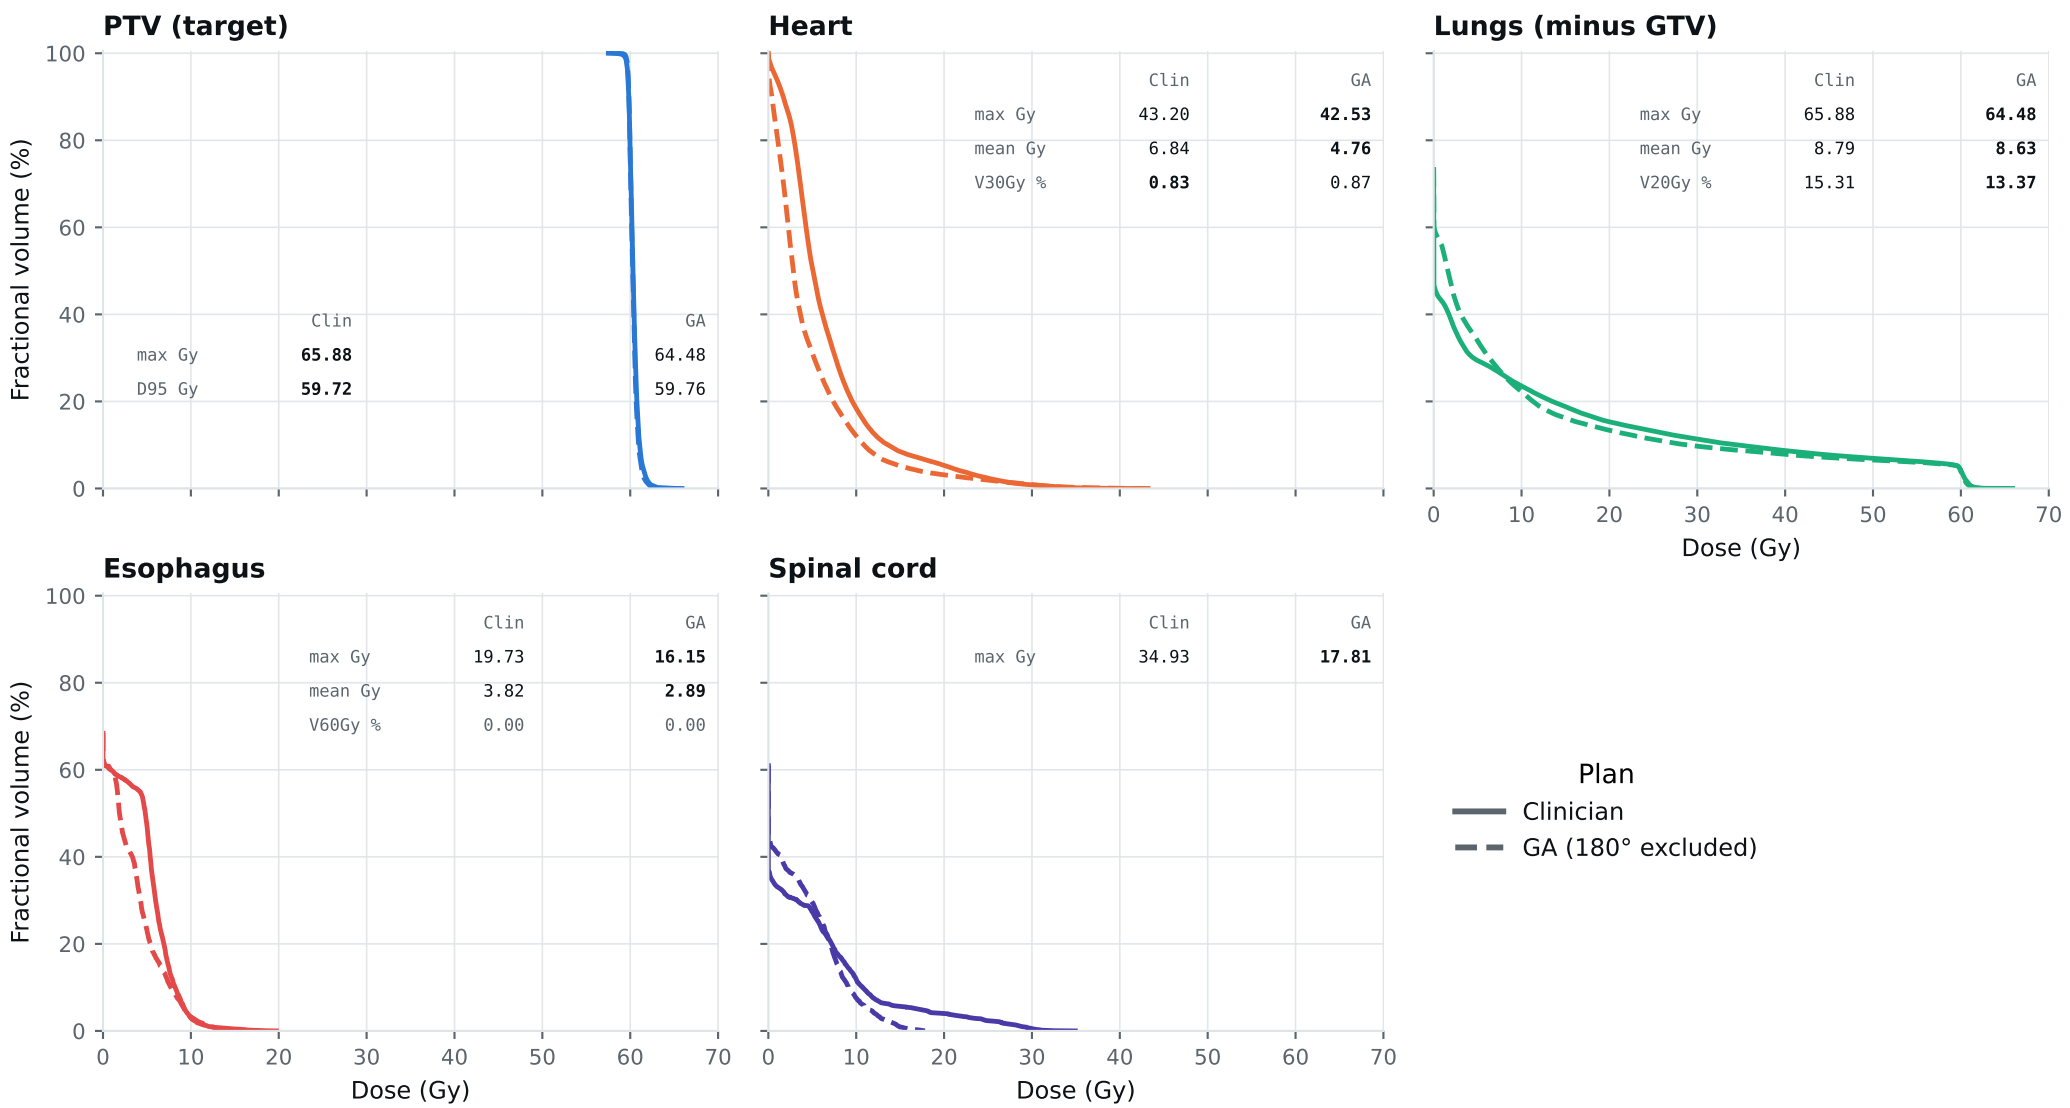

Clinical criteria — Lung_Patient_11

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	63.06	62.12	Gy
PTV max	69	66	65.88	64.48	Gy
ESOPHAGUS max	66	—	19.73	16.15	Gy
ESOPHAGUS mean	34	21	3.82	2.89	Gy
ESOPHAGUS V60Gy	17	—	0.00	0.00	%
HEART max	66	—	43.20	42.53	Gy
HEART mean	27	20	6.84	4.76	Gy
HEART V30Gy	50	48	0.83	0.87	%
LUNG_L max	66	—	10.29	25.80	Gy
LUNG_R max	66	—	65.88	64.48	Gy
CORD max	50	48	34.93	17.81	Gy
SKIN max	60	—	51.63	51.50	Gy
LUNGS_NOT_GTV max	66	—	65.88	64.48	Gy
LUNGS_NOT_GTV mean	21	20	8.79	8.63	Gy
LUNGS_NOT_GTV V20Gy	37	—	15.31	13.37	%
PTV D95 (target coverage)			59.72	59.76	
Objective value (search signal)			58.63	52.08	
Pipeline time (setup + solve)			30 s	39 s	
Beam angles (gantry°)	Clinician	147°, 355°, 340°, 315°, 235°, 205°, 185°			
	GA	205°, 185°, 120°, 165°, 240°, 270°, 285°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_11_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.