





Dose-volume histogram — Lung_Patient_17

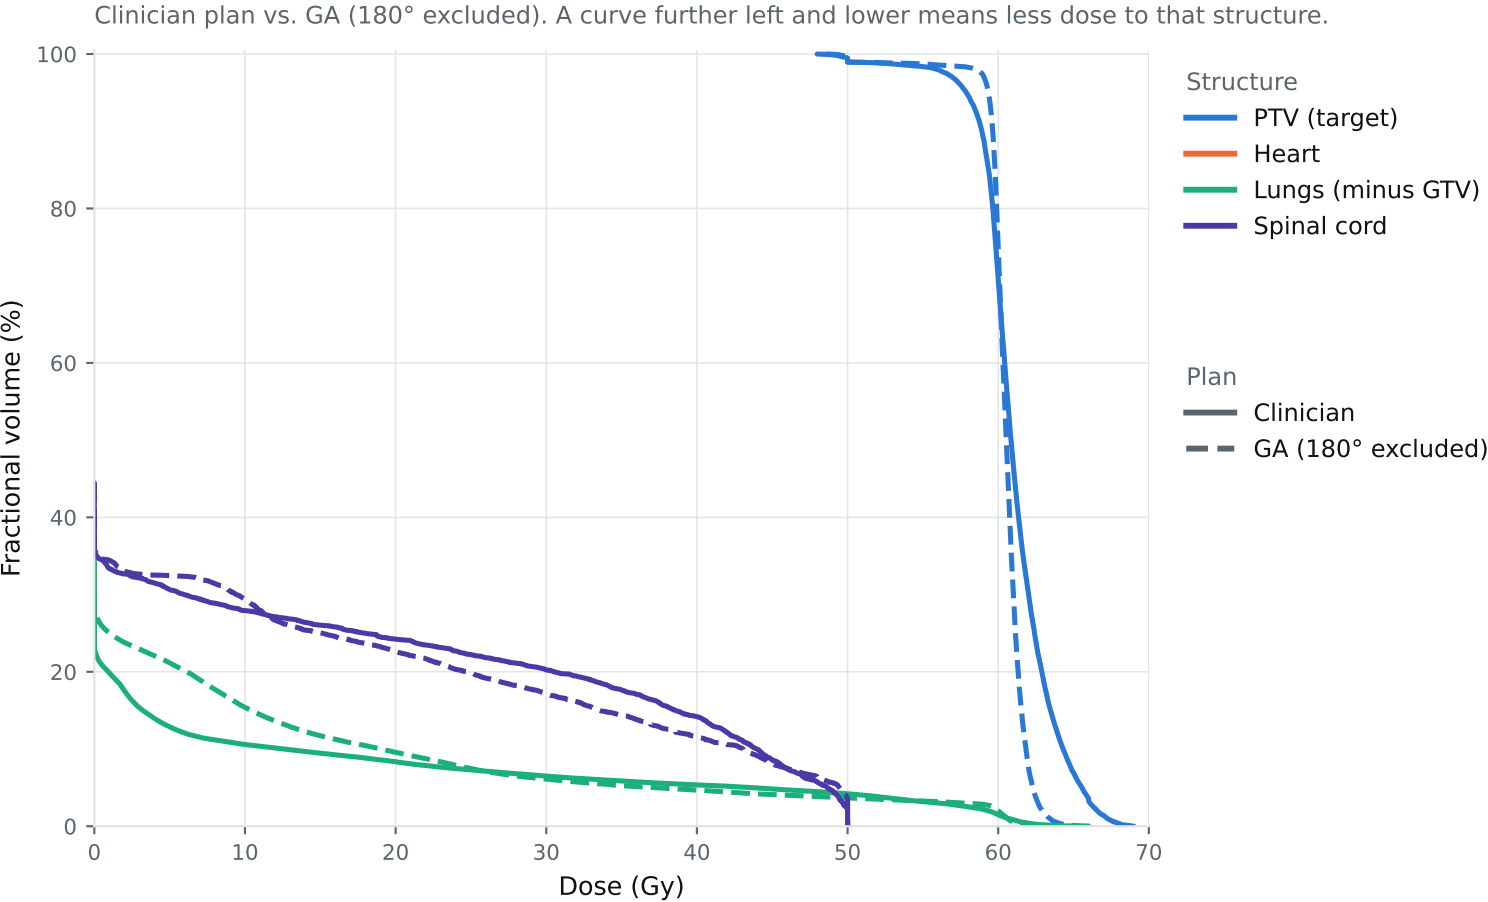

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_17

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

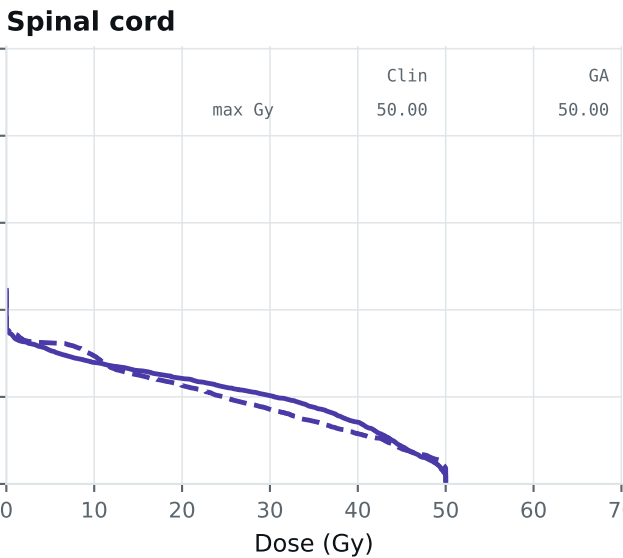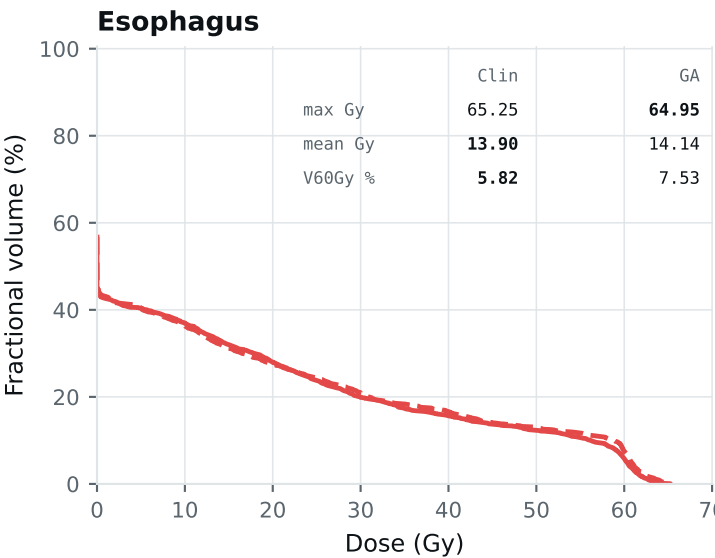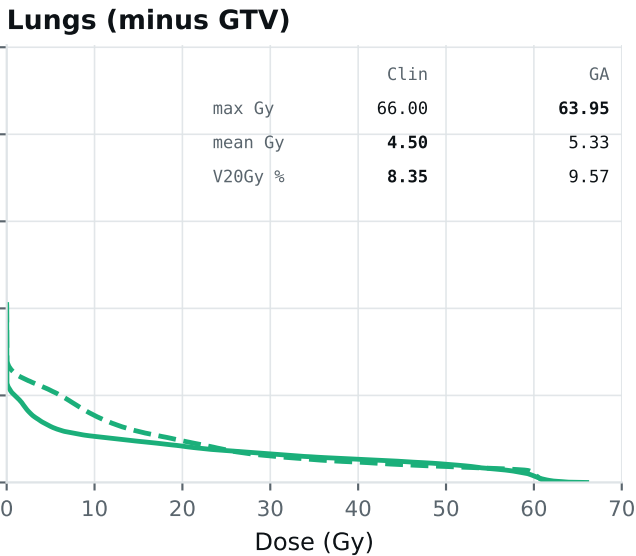

Plan

- Clinician
- GA (180° excluded)

Clinical criteria — Lung_Patient_17

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	69.00	64.79	Gy
PTV max	69	66	69.00	66.05	Gy
ESOPHAGUS max	66	—	65.25	64.95	Gy
ESOPHAGUS mean	34	21	13.90	14.14	Gy
ESOPHAGUS V60Gy	17	—	5.82	7.53	%
HEART max	66	—	0.00	0.00	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	37.63	43.45	Gy
LUNG_R max	66	—	66.00	63.95	Gy
CORD max	50	48	50.00	50.00	Gy
SKIN max	60	—	52.16	48.63	Gy
LUNGS_NOT_GTV max	66	—	66.00	63.95	Gy
LUNGS_NOT_GTV mean	21	20	4.50	5.33	Gy
LUNGS_NOT_GTV V20Gy	37	—	8.35	9.57	%
PTV D95 (target coverage)			57.90	59.36	
Objective value (search signal)			413.09	275.57	
Pipeline time (setup + solve)			48 s	40 s	
Beam angles (gantry°)	Clinician	152°, 20°, 0°, 318°, 236°, 208°, 185°			
	GA	20°, 0°, 236°, 75°, 120°, 165°, 300°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_17_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.