



Dose-volume histogram — Lung_Patient_21

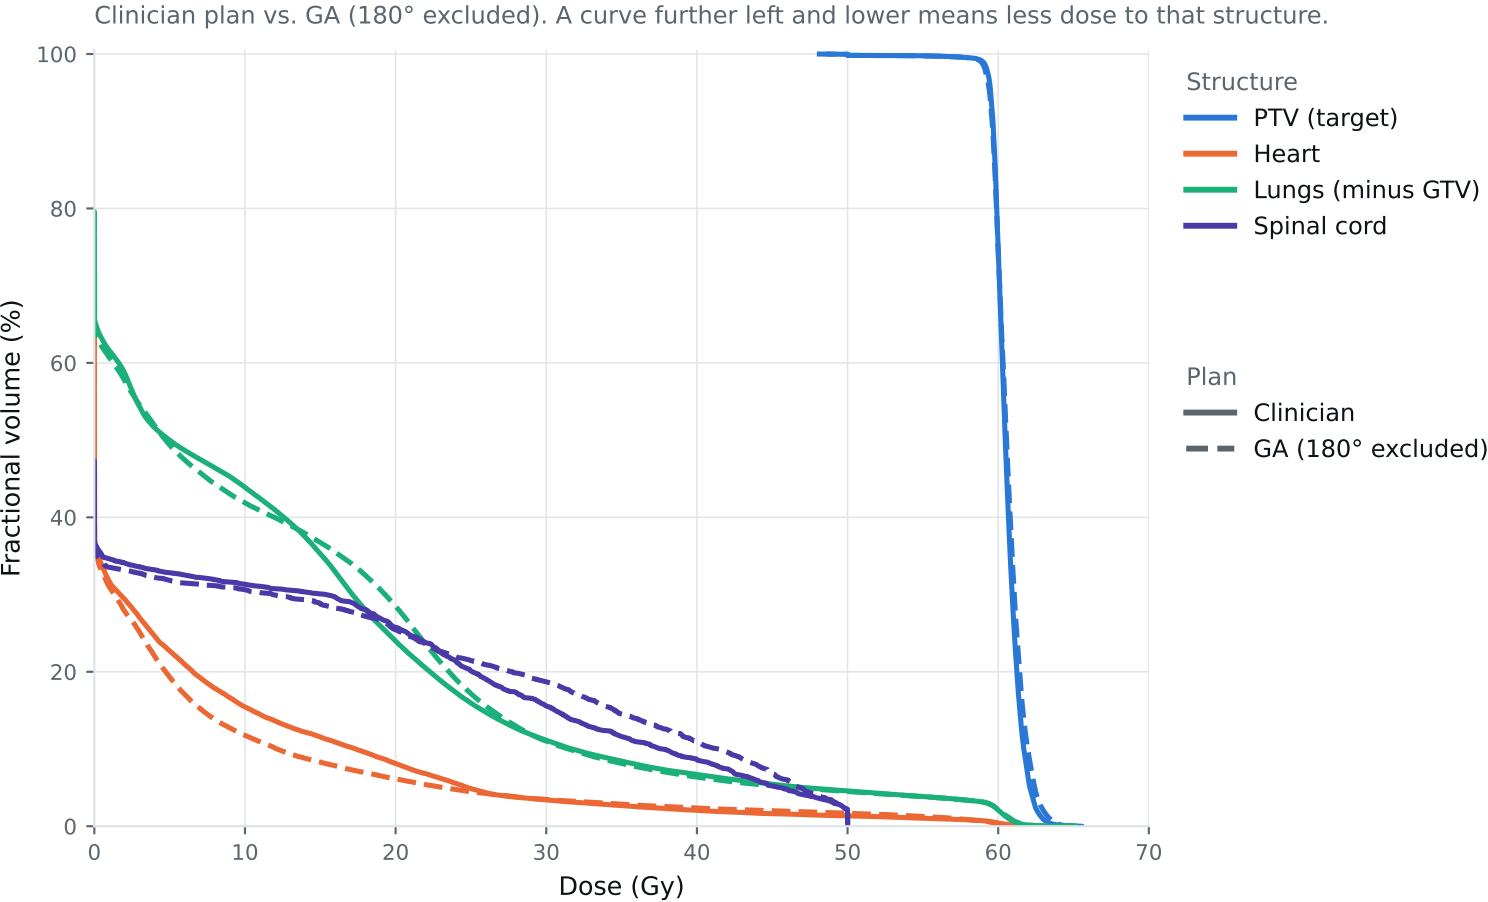

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_21

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

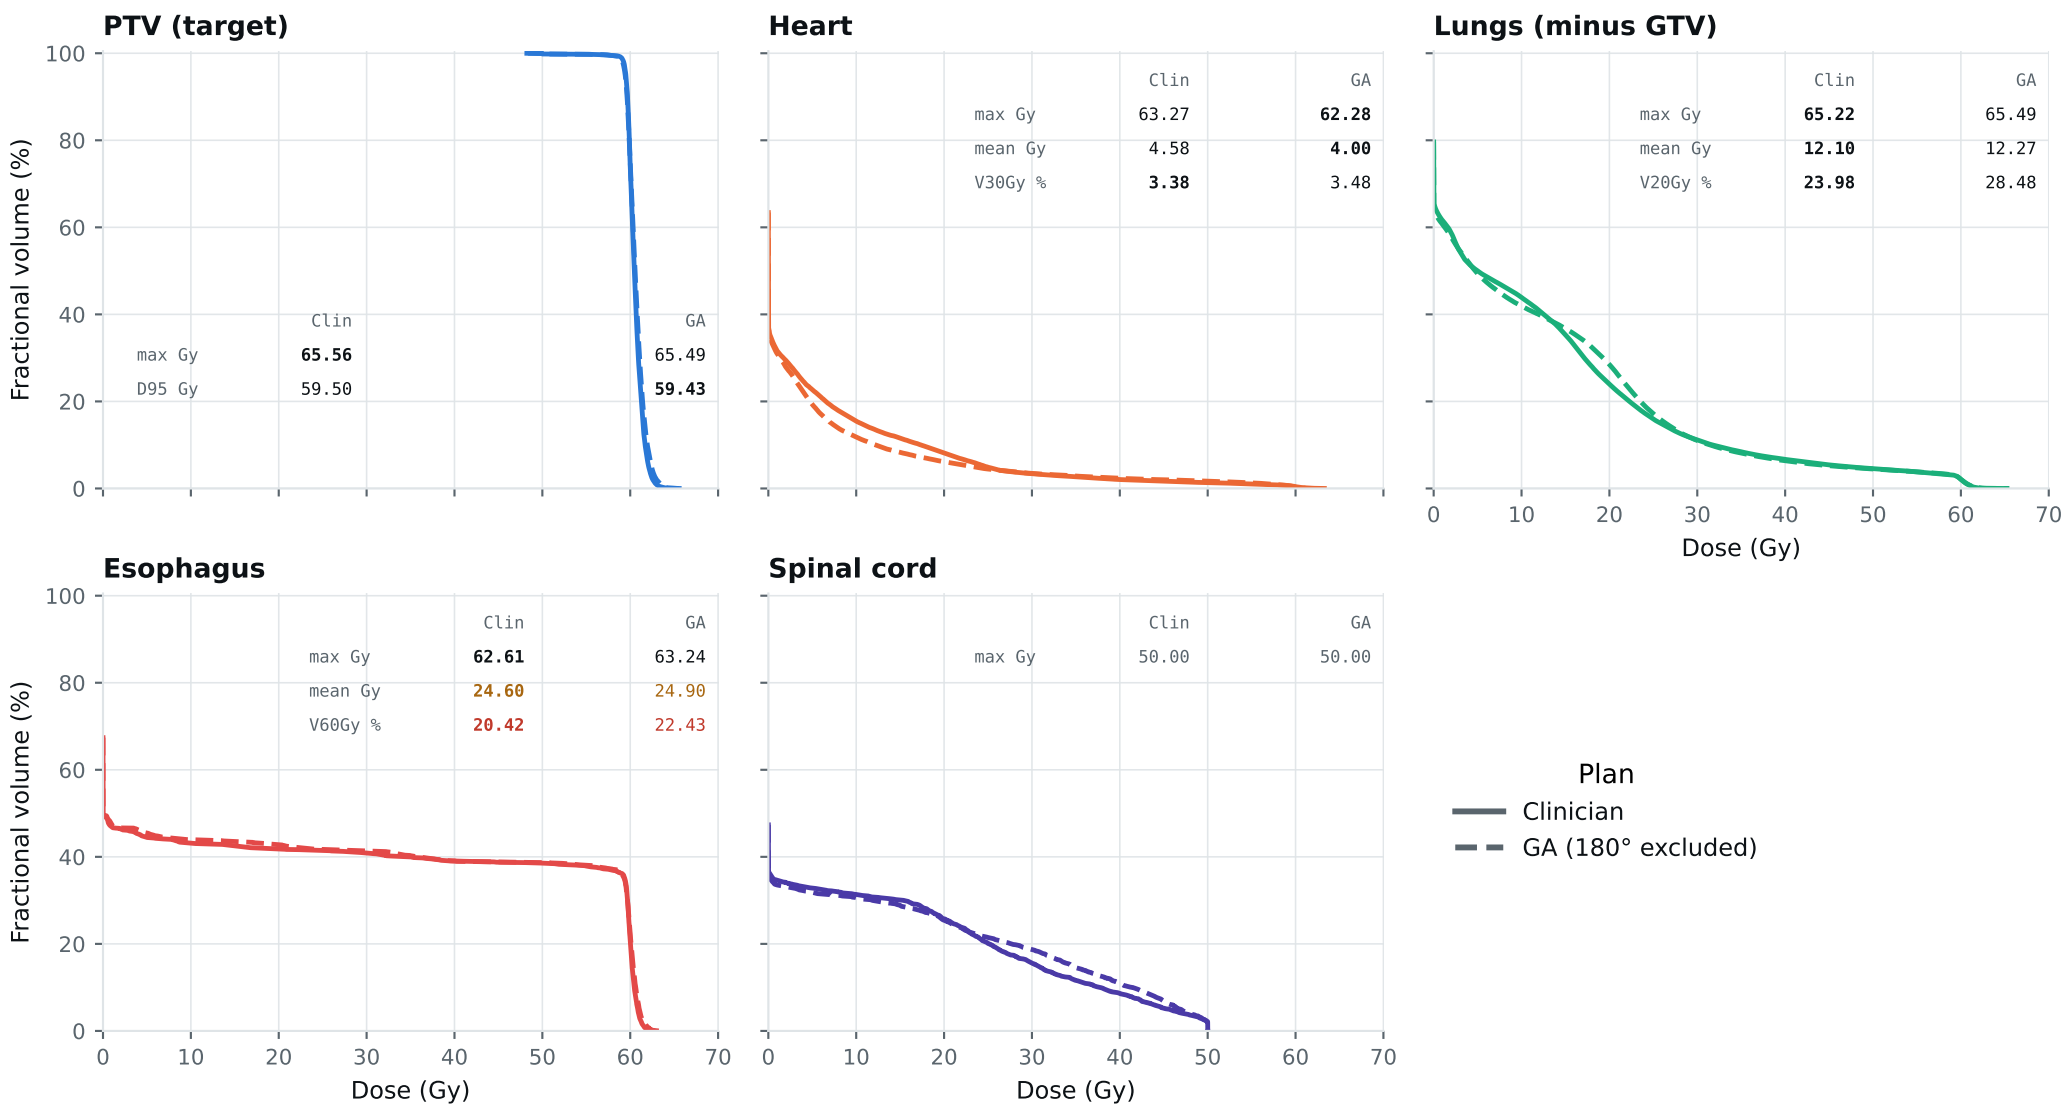

Clinical criteria — Lung_Patient_21

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	64.44	65.08	Gy
PTV max	69	66	65.56	65.49	Gy
ESOPHAGUS max	66	—	62.61	63.24	Gy
ESOPHAGUS mean	34	21	24.60	24.90	Gy
ESOPHAGUS V60Gy	17	—	20.42	22.43	%
HEART max	66	—	63.27	62.28	Gy
HEART mean	27	20	4.58	4.00	Gy
HEART V30Gy	50	48	3.38	3.48	%
LUNG_L max	66	—	63.01	62.65	Gy
LUNG_R max	66	—	65.22	65.49	Gy
CORD max	50	48	50.00	50.00	Gy
SKIN max	60	—	50.01	46.97	Gy
LUNGS_NOT_GTV max	66	—	65.22	65.49	Gy
LUNGS_NOT_GTV mean	21	20	12.10	12.27	Gy
LUNGS_NOT_GTV V20Gy	37	—	23.98	28.48	%
PTV D95 (target coverage)			59.50	59.43	
Objective value (search signal)			172.43	179.84	
MOSEK solve time			75 s	61 s	
Beam angles (gantry°)	Clinician	175°, 143°, 110°, 45°, 0°, 315°, 248°, 210°			
	GA	210°, 75°, 135°, 165°, 195°, 285°, 345°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_21_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.