



Dose-volume histogram — Lung_Patient_7

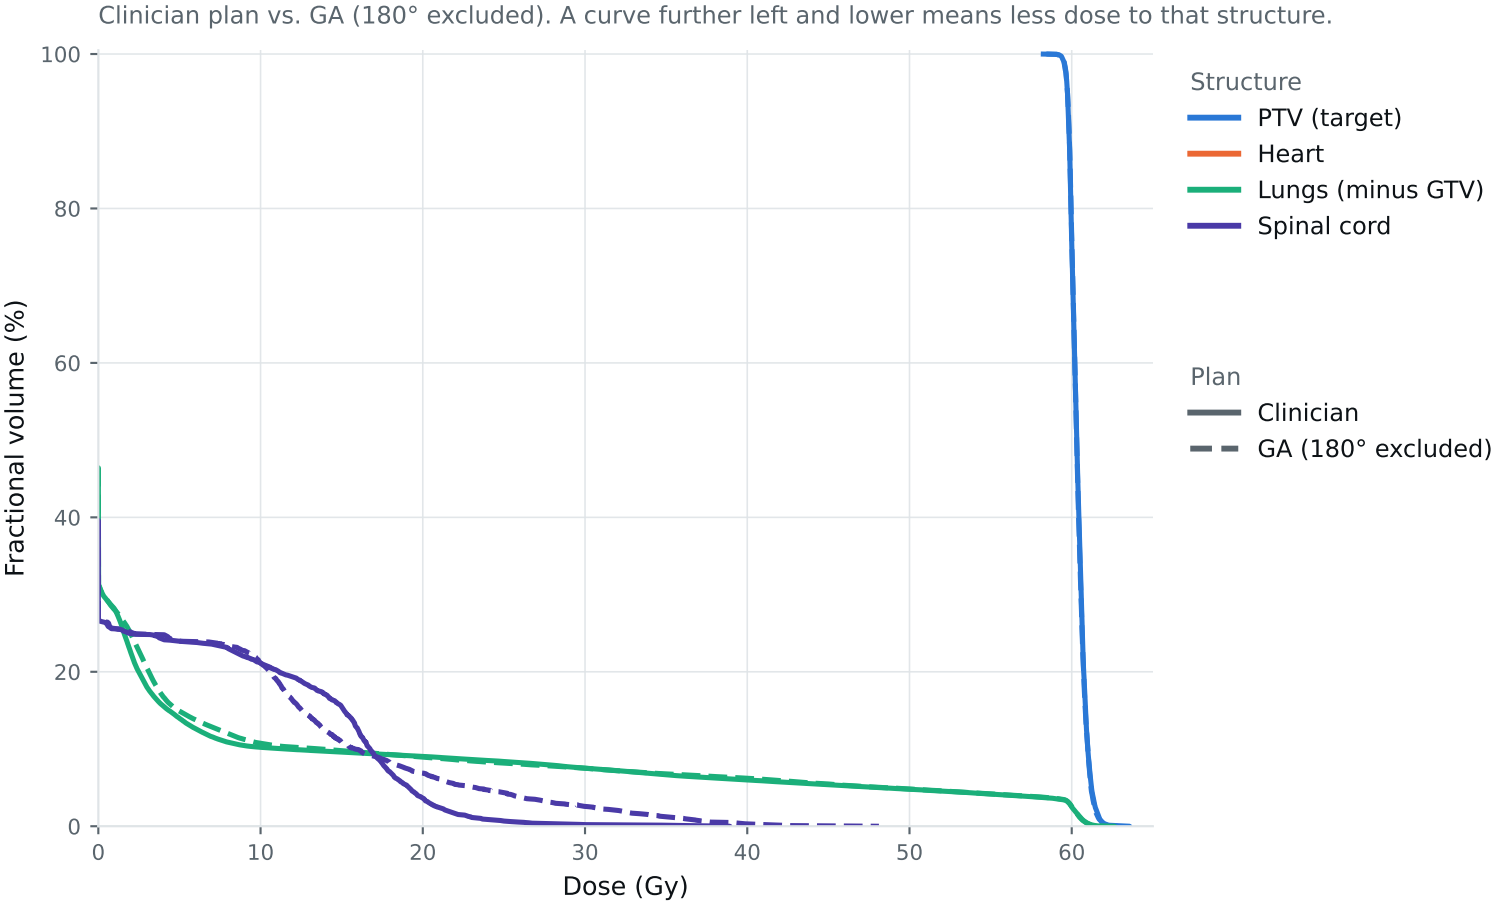

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_7

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

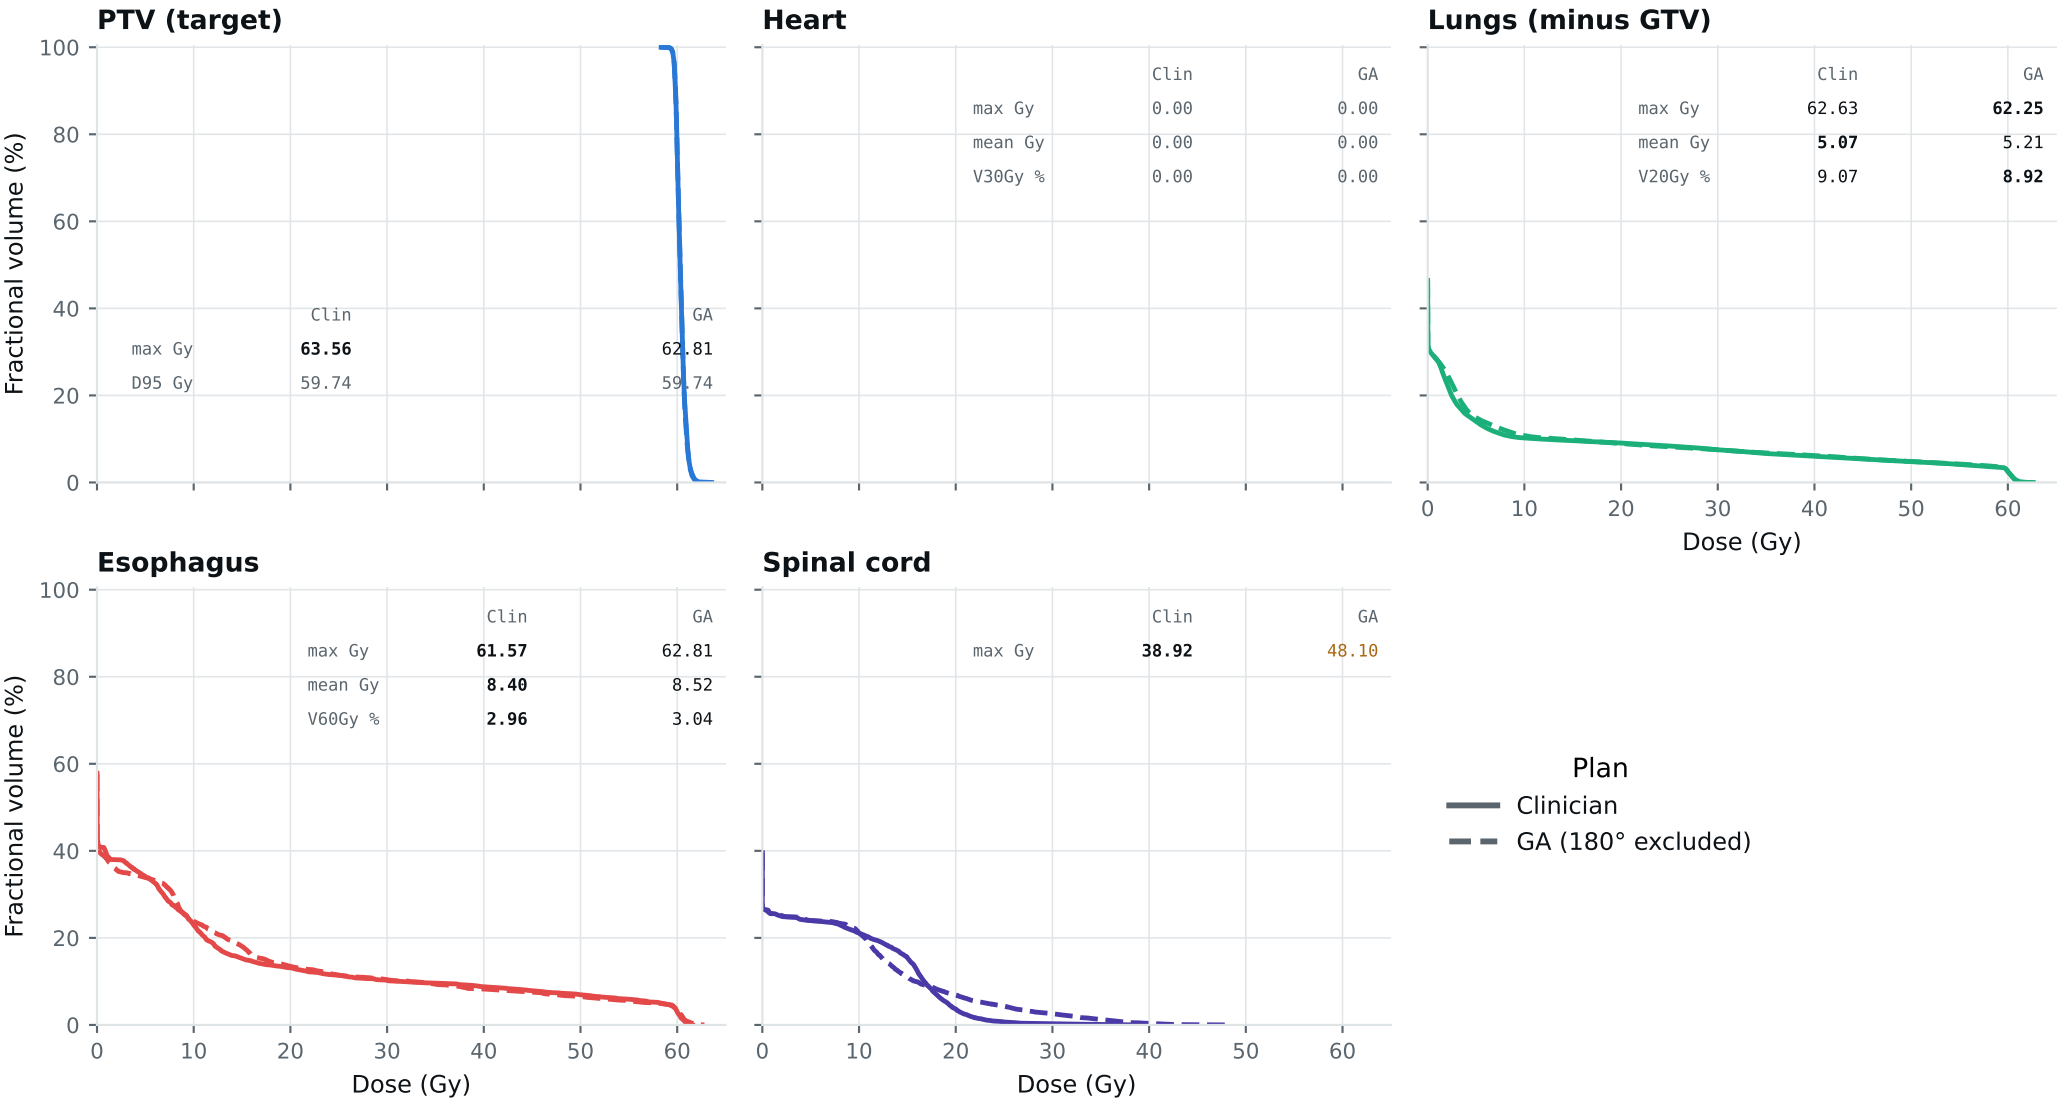

Clinical criteria — Lung_Patient_7

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.26	61.93	Gy
PTV max	69	66	63.56	62.81	Gy
ESOPHAGUS max	66	—	61.57	62.81	Gy
ESOPHAGUS mean	34	21	8.40	8.52	Gy
ESOPHAGUS V60Gy	17	—	2.96	3.04	%
HEART max	66	—	0.00	0.00	Gy
HEART mean	27	20	0.00	0.00	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	14.84	21.61	Gy
LUNG_R max	66	—	62.63	62.25	Gy
CORD max	50	48	38.92	48.10	Gy
SKIN max	60	—	45.00	44.43	Gy
LUNGS_NOT_GTV max	66	—	62.63	62.25	Gy
LUNGS_NOT_GTV mean	21	20	5.07	5.21	Gy
LUNGS_NOT_GTV V20Gy	37	—	9.07	8.92	%
PTV D95 (target coverage)			59.74	59.74	
Objective value (search signal)			66.92	67.81	
Pipeline time (setup + solve)			20 s	20 s	
Beam angles (gantry°)	Clinician	0°, 185°, 210°, 240°, 270°, 300°, 330°			
	GA	15°, 45°, 165°, 185°, 255°, 285°, 315°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_7_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.