







Dose-volume histogram — Lung_Patient_9

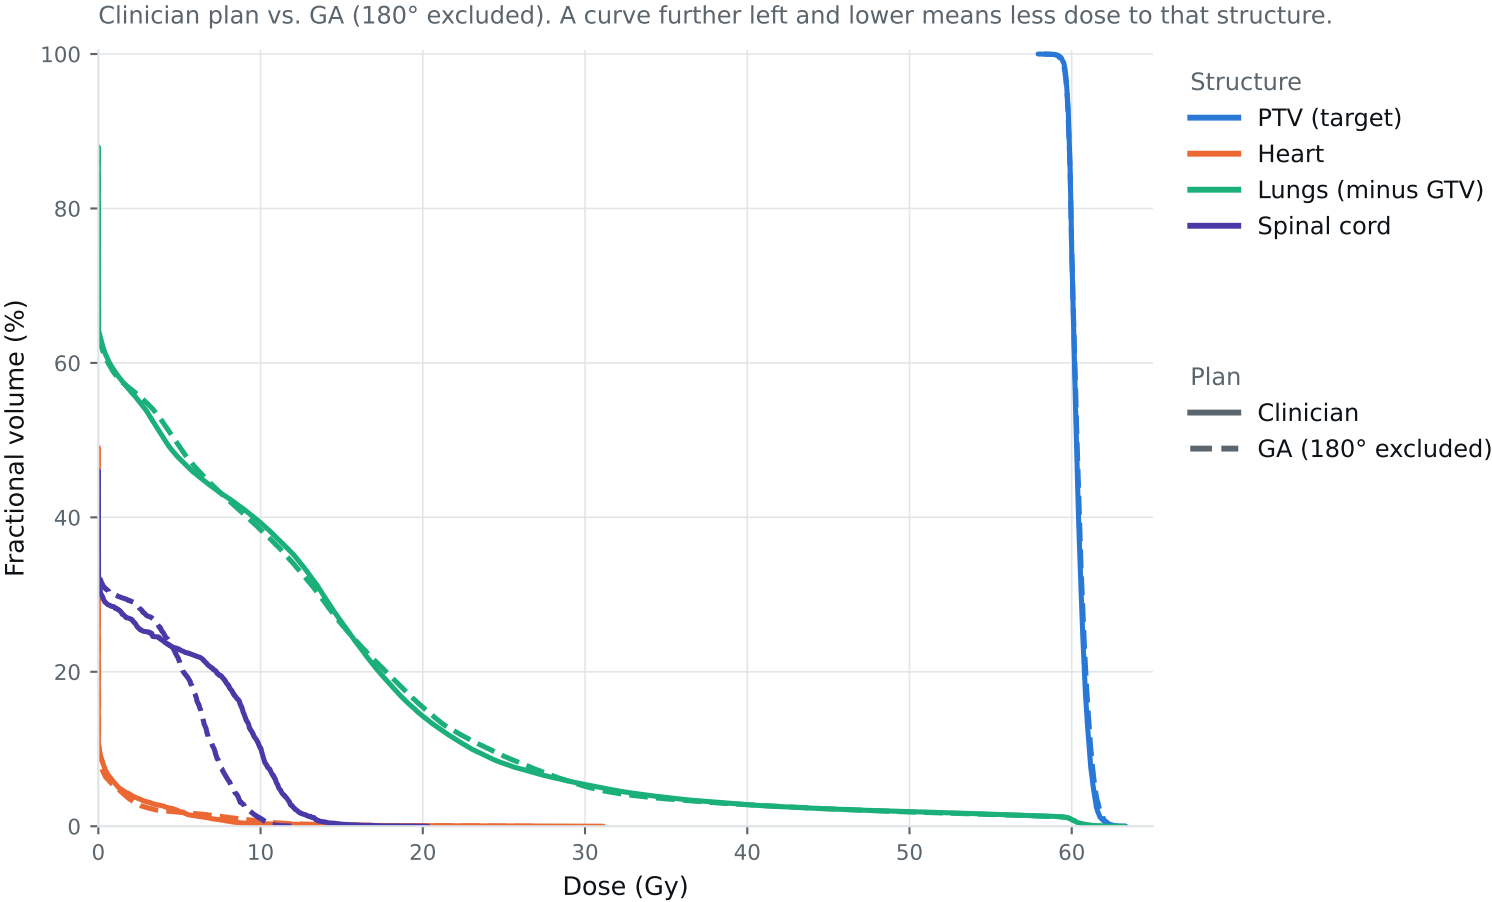

Curves further left are better for organs; the PTV curve should stay high, then drop sharply. Target curves should overlap; organ curves show the tradeoffs. Esophagus is on page 2.

DVH by structure — Lung_Patient_9

Same curves, one structure per panel, all plans, each annotated with that structure's protocol metrics.
Bold = clinically preferable: organs favor lower dose; PTV favors the value closest to goal within the limit. Grey = all plans are within 0.01 of each other. Amber misses a goal,

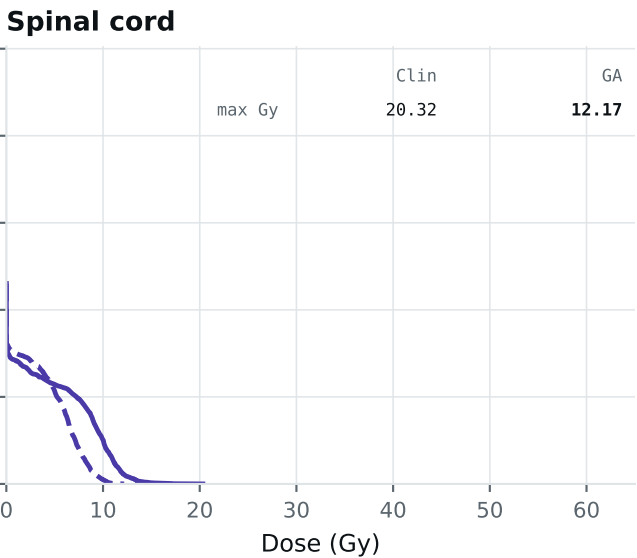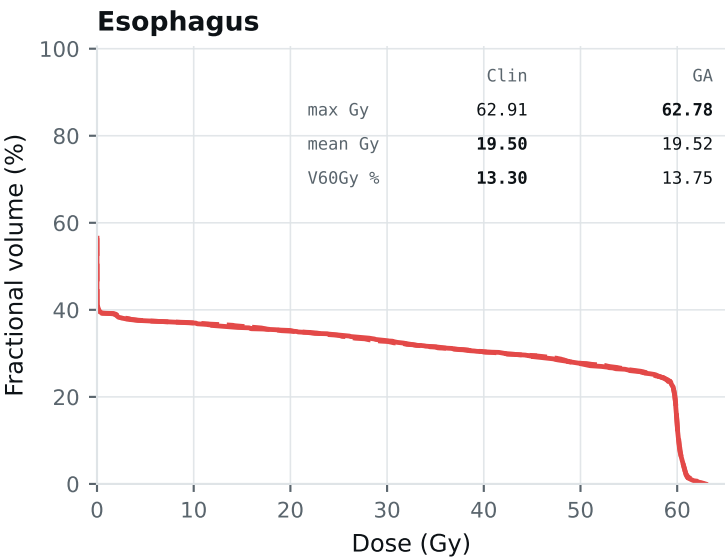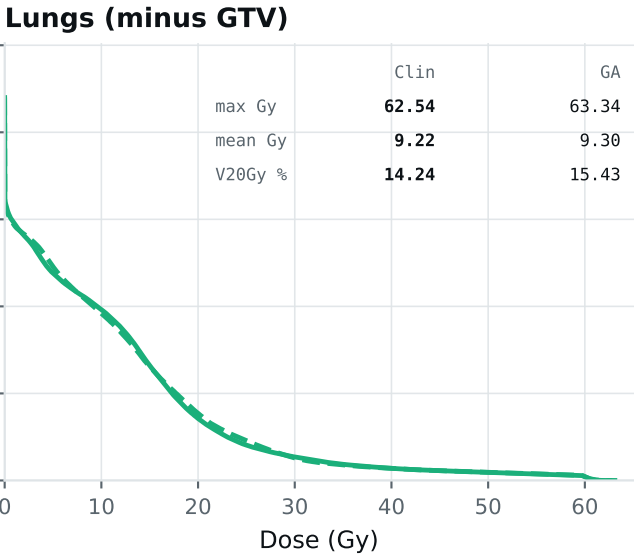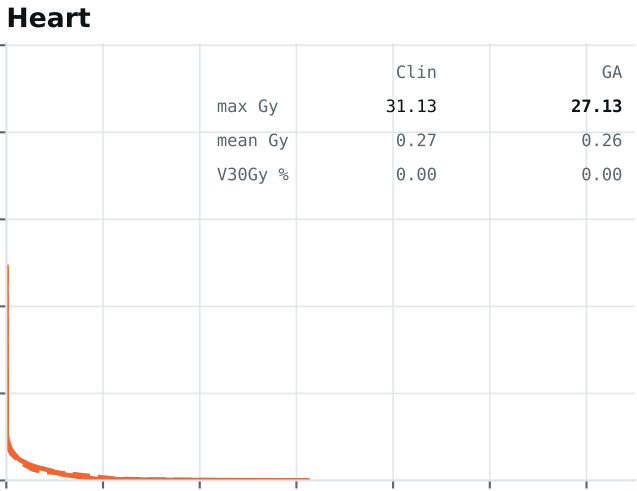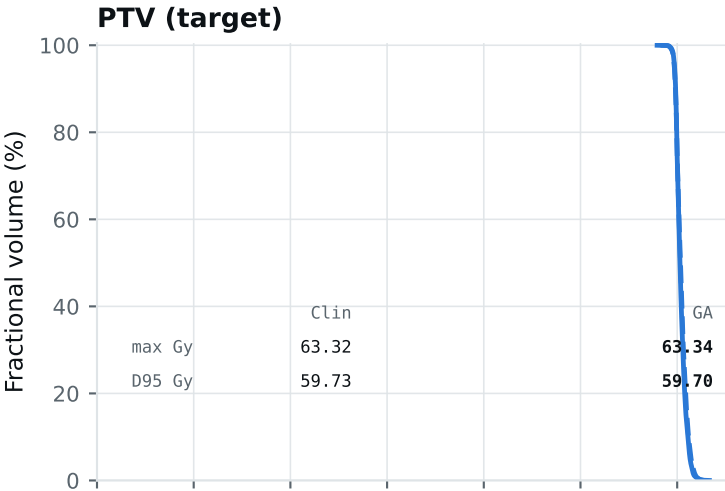

Plan
— Clinician
- - GA (180° excluded)

Clinical criteria — Lung_Patient_9

Organs: lower is better. PTV: closest to goal without exceeding the limit. Bold marks the best plan.

Criterion	Limit	Goal	Clinician	GA 180° excluded	
GTV max	69	66	62.08	62.04	Gy
PTV max	69	66	63.32	63.34	Gy
ESOPHAGUS max	66	—	62.91	62.78	Gy
ESOPHAGUS mean	34	21	19.50	19.52	Gy
ESOPHAGUS V60Gy	17	—	13.30	13.75	%
HEART max	66	—	31.13	27.13	Gy
HEART mean	27	20	0.27	0.26	Gy
HEART V30Gy	50	48	0.00	0.00	%
LUNG_L max	66	—	60.20	60.81	Gy
LUNG_R max	66	—	62.54	63.34	Gy
CORD max	50	48	20.32	12.17	Gy
SKIN max	60	—	41.34	42.31	Gy
LUNGS_NOT_GTV max	66	—	62.54	63.34	Gy
LUNGS_NOT_GTV mean	21	20	9.22	9.30	Gy
LUNGS_NOT_GTV V20Gy	37	—	14.24	15.43	%
PTV D95 (target coverage)			59.73	59.70	
Objective value (search signal)			84.77	85.93	
Pipeline time (setup + solve)			35 s	24 s	
Beam angles (gantry°)	Clinician	0°, 50°, 100°, 140°, 175°, 220°, 260°, 310°			
	GA	0°, 90°, 120°, 210°, 240°, 310°, 345°			

Grey rows: all plans agree within 0.01 — heart, lung and LUNGS_NOT_GTV max sit at 66 Gy because those structures abut the target. Amber misses the goal; red exceeds the limit.

Source: Lung_Patient_9_clinical_metrics_full_resolution.json, full resolution. The curves and table come from the same solve.