

Certificate No. 34159/DBBPAM  
Date: September 30, 2019



Issuing Office:  
Jl. Arteri Tol Cibitung No. 1, Cibitung Bekasi 17520, Indonesia  
Phone/Facs: +62 21 88321176/88321166  
Email: jum.cbt@sucofindo.co.id

## CERTIFICATE OF CALIBRATION

CLIENT : SENTRAL TEHNOLOGY MANAGEMEN, PT  
ADDRESS : CIKARANG SQUARE BLOK B NO. 11  
JL. RAYA CIBARUSAH CIKARANG SELATAN  
CIKARANG - JAWA BARAT

NAME OF EQUIPMENT : ANAK TIMBANGAN

SERIAL NO. / CODE : - / CSM-014

MATERIALS : STAINLESS STEEL

WEIGHT / CLASS : 1 mg ~ 200 g / F1


MANUFACTURER : EXCELLENT

The Attachment available is an integral part of this certificate.

This calibration result (s) related to the sample (s) submitted only and the certificate cannot be reproduced in any way, except in full context and with the prior approval in writing from Sucofindo Laboratory.

This Certificate/report is issued under our General Terms and Conditions, copy of which is available upon request or may be accessed at [www.sucofindo.co.id](http://www.sucofindo.co.id)

CBT200295119-001

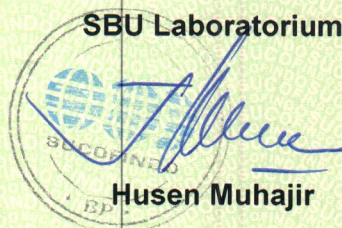

3328098

SCI-2007A



Amendment No. AM 134/DBBPAM  
Date: October 14, 2019



Issuing Office:  
Jl. Arteri Tol Cibitung No. 1, Cibitung Bekasi 17520, Indonesia  
Phone/Facs: +62 21 88321176/88321166  
Email: jum.cbt@sucofindo.co.id

## AMENDMENT TO CERTIFICATE NO. 34159/DBBPAM DATE: SEPTEMBER 30, 2019

### WRITTEN

Page 1 :  
CLIENT : SENTRAL TEHNOLOGY MANAGEMEN, PT  
Page 2 :

NOMINAL	CONVENTIONAL MASS	UNCERTAINTY OF MEASUREMENT at 95% Confidence Level	k =
mg	mg	mg	
500	499.992	0.027	2.00
200	200.007	0.020	2.00
200 *	199.998	0.020	2.00
100	100.009	0.017	1.99
50	49.994	0.013	2.00
20	20.006	0.010	1.99
20 *	20.001	0.010	2.00
10	10.010	0.0083	1.98
5	5.006	0.0067	1.98
2	2.004	0.0067	1.98
2 *	0.205	0.0067	1.98
1	1.006	0.0067	1.99

### SHOULD READ


CLIENT : SENTRAL TEHNOLOGI MANAGEMEN, PT

NOMINAL	CONVENTIONAL MASS	UNCERTAINTY OF MEASUREMENT at 95% Confidence Level	k =
mg	mg	mg	
500	499.992	0.027	2.00
200	200.007	0.020	2.00
200 *	199.998	0.020	2.00
100	100.009	0.017	1.99
50	49.994	0.013	2.00
20	20.006	0.010	1.99
20 *	20.001	0.010	2.00
10	10.010	0.0083	1.98
5	5.006	0.0067	1.98
2	2.004	0.0067	1.98
2 *	2.003	0.0067	1.98
1	1.006	0.0067	1.99

All other matters in the certificate remain unchanged.

This calibration result (s) related to the sample (s) submitted only and the certificate cannot be reproduced in any way, except in full context and with the prior approval in writing from Sucofindo Laboratory.

This Certificate/report is issued under our General Terms and Conditions, copy of which is available upon request or may be accessed at [www.sucofindo.co.id](http://www.sucofindo.co.id)

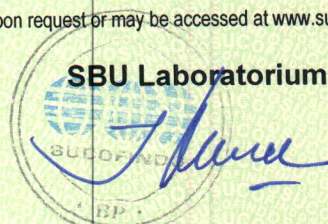

Husen Muhajir

CBT200295119-001



3346105

SCI-2007A