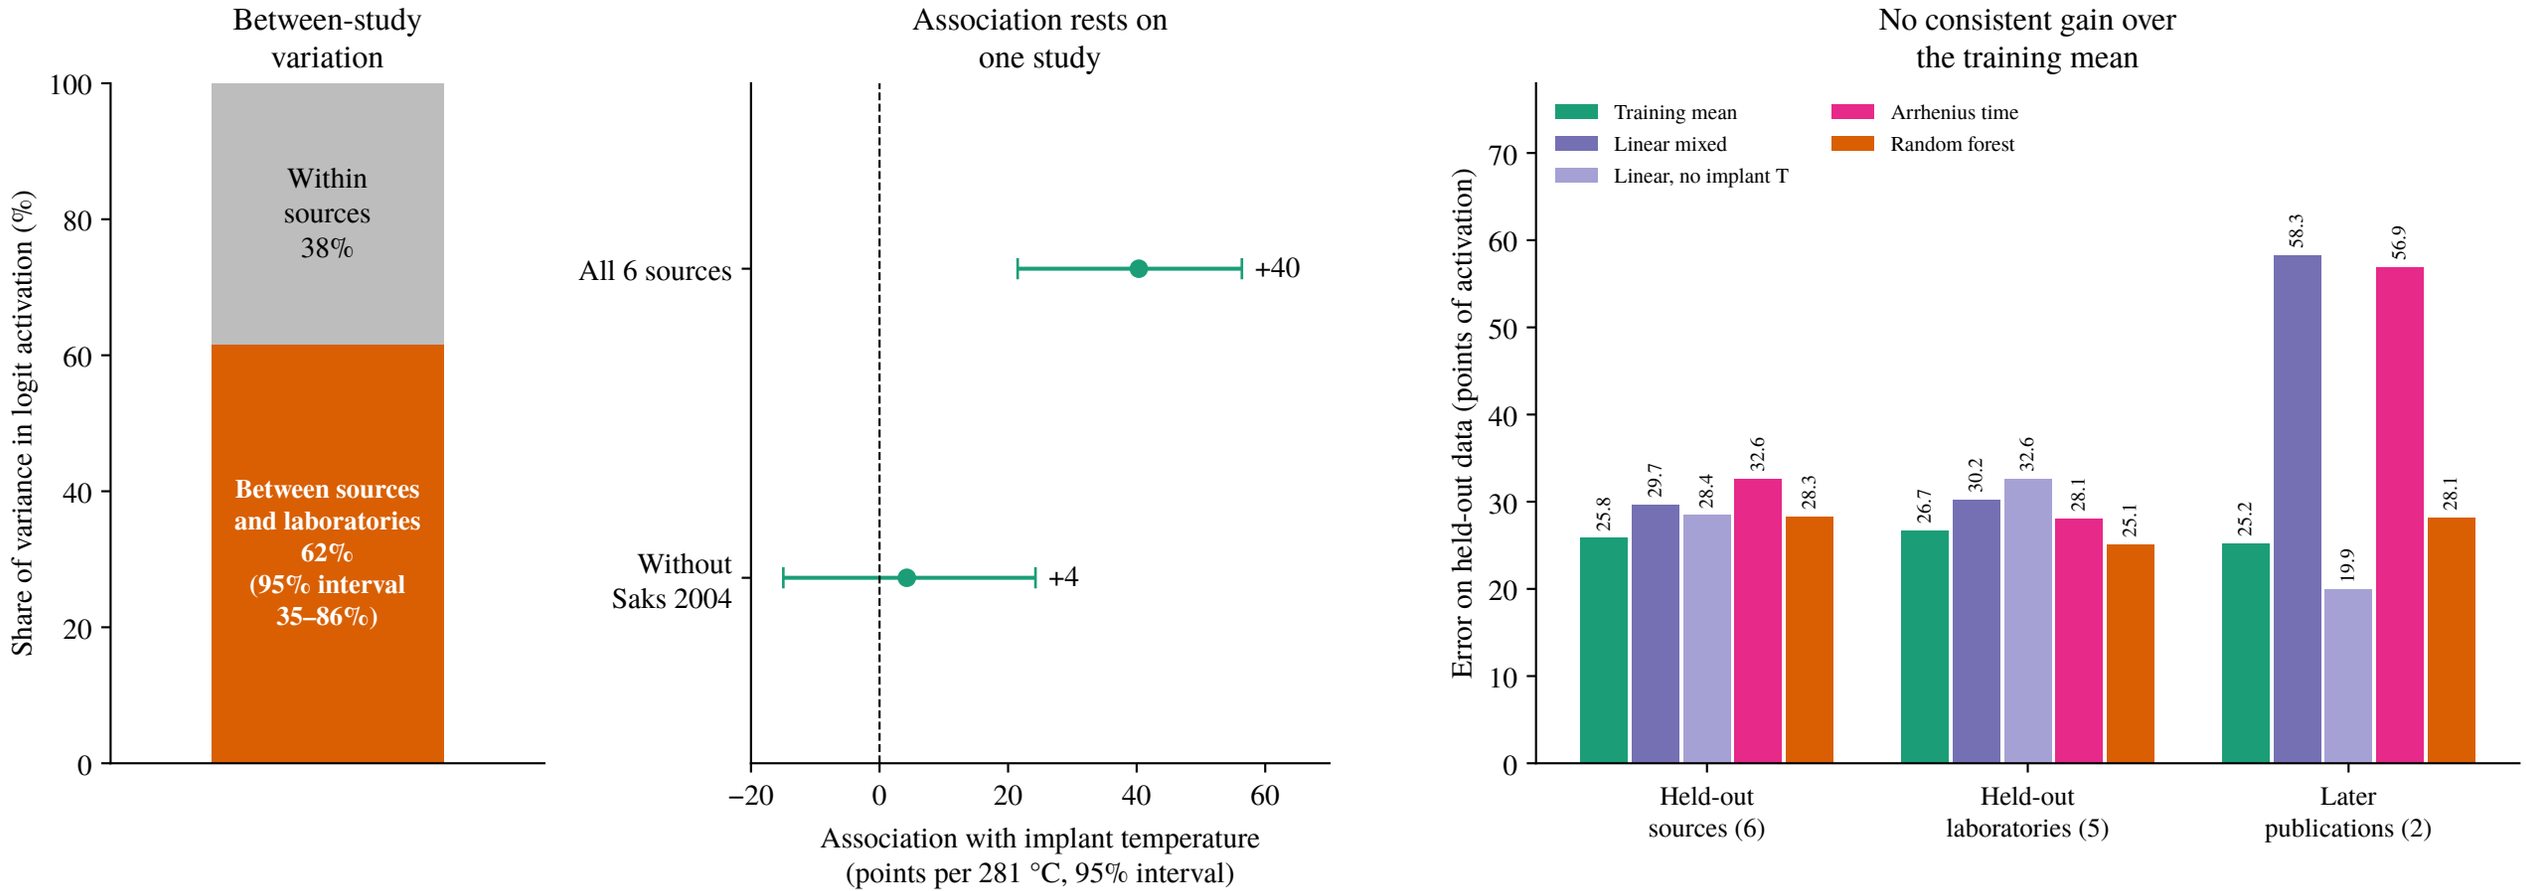
Between-study variation
Share of variance in logit activation (%)
100
80
60
40
20
0
Within sources 38%
Between sources and laboratories 62% (95% interval 35–86%)
Association rests on one study
All 6 sources
+40
Without Saks 2004
+4
−20
0
20
40
60
Association with implant temperature (points per 281 °C, 95% interval)
No consistent gain over the training mean
Error on held-out data (points of activation)
70
60
50
40
30
20
10
0
Training mean
Linear mixed
Linear, no implant T
Arrhenius time
Random forest
25.8
29.7
28.4
32.6
28.3
26.7
30.2
32.6
28.1
25.1
25.2
58.3
19.9
56.9
28.1
Held-out sources (6)
Held-out laboratories (5)
Later publications (2)