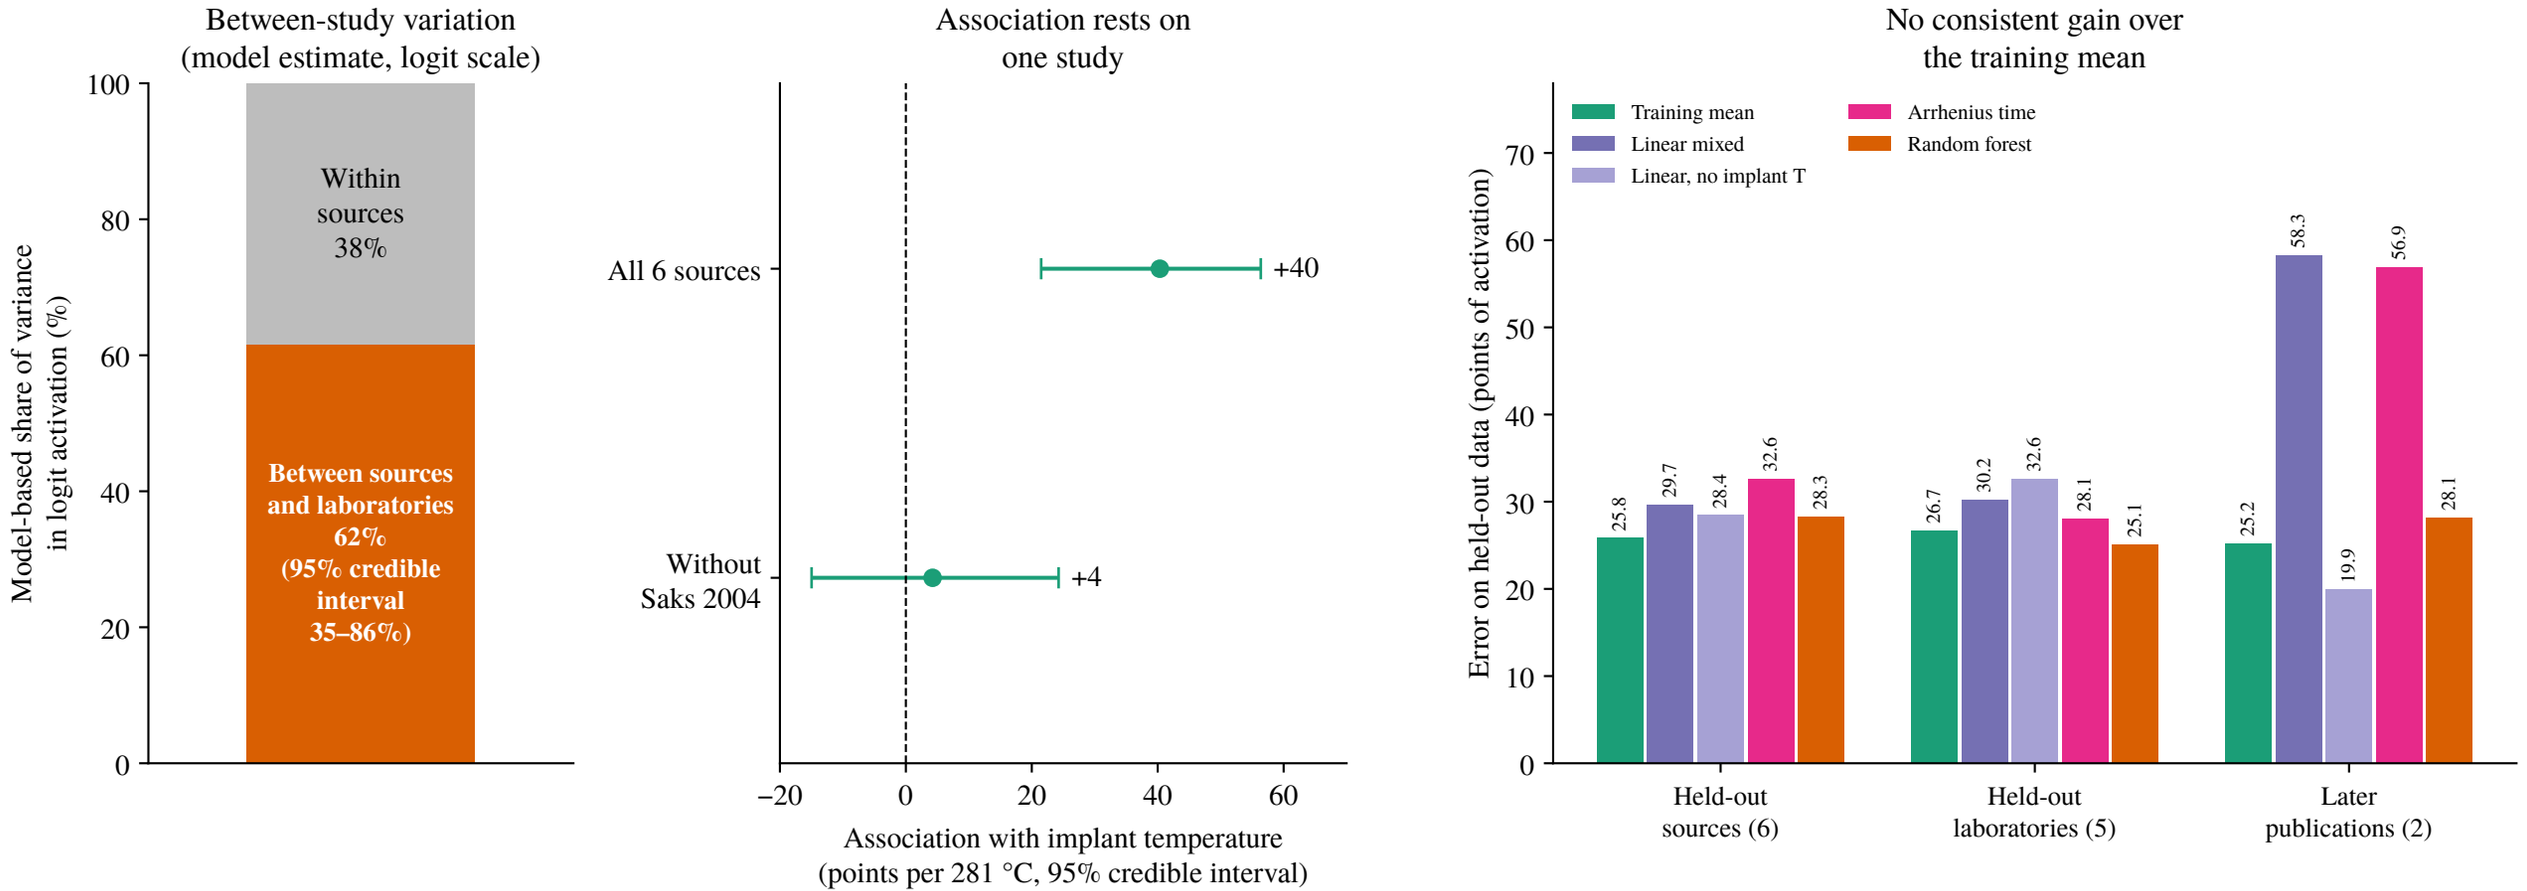
Between-study variation
(model estimate, logit scale)
Model-based share of variance
in logit activation (%)
100
80
60
40
20
0
Within
sources
38%
Between sources
and laboratories
62%
(95% credible
interval
35–86%)
Association rests on
one study
All 6 sources
+40
Without
Saks 2004
+4
−20
0
20
40
60
Association with implant temperature
(points per 281 °C, 95% credible interval)
No consistent gain over
the training mean
Error on held-out data (points of activation)
Training mean
Linear mixed
Linear, no implant T
Arrhenius time
Random forest
70
60
50
40
30
20
10
0
25.8
29.7
28.4
32.6
28.3
26.7
30.2
32.6
28.1
25.1
25.2
58.3
19.9
56.9
28.1
Held-out
sources (6)
Held-out
laboratories (5)
Later
publications (2)