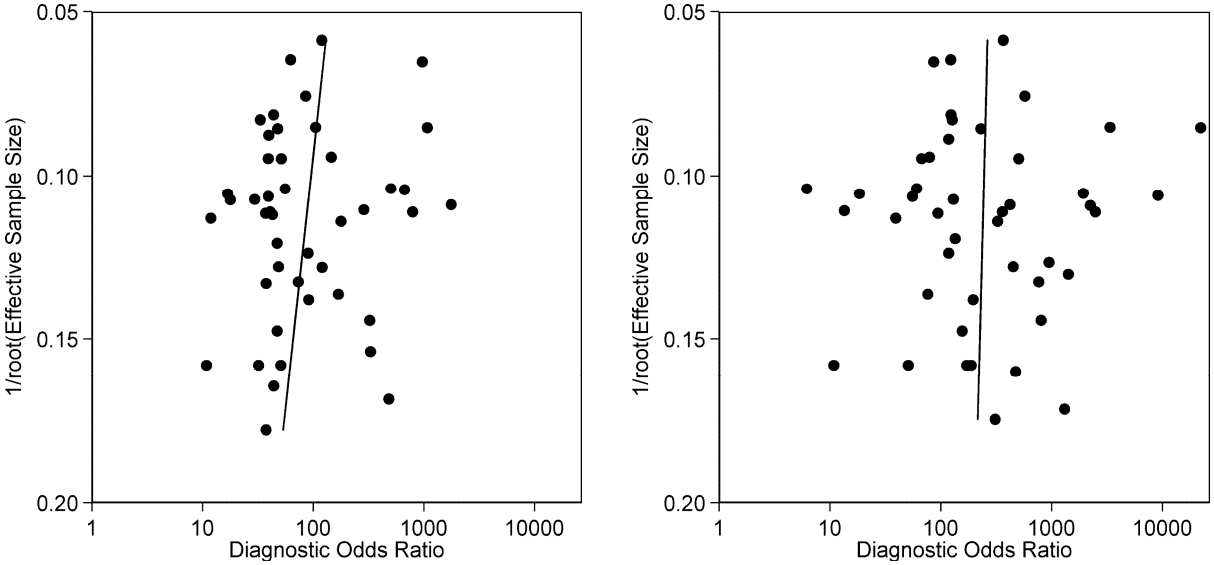S2 Fig. Deek's funnel plot assessment test for assessing any potential publication bias among studies evaluating pleural fluid adenosine deaminase (left panel) and unstimulated interferon-gamma (right panel). Both these plots show a symmetric distribution of the log of diagnostic odds ratios against inverse root of effective sample sizes, indicating absence of any significant publication bias for either assay.