


Nightlight Sensor Comparison in Overlap Period

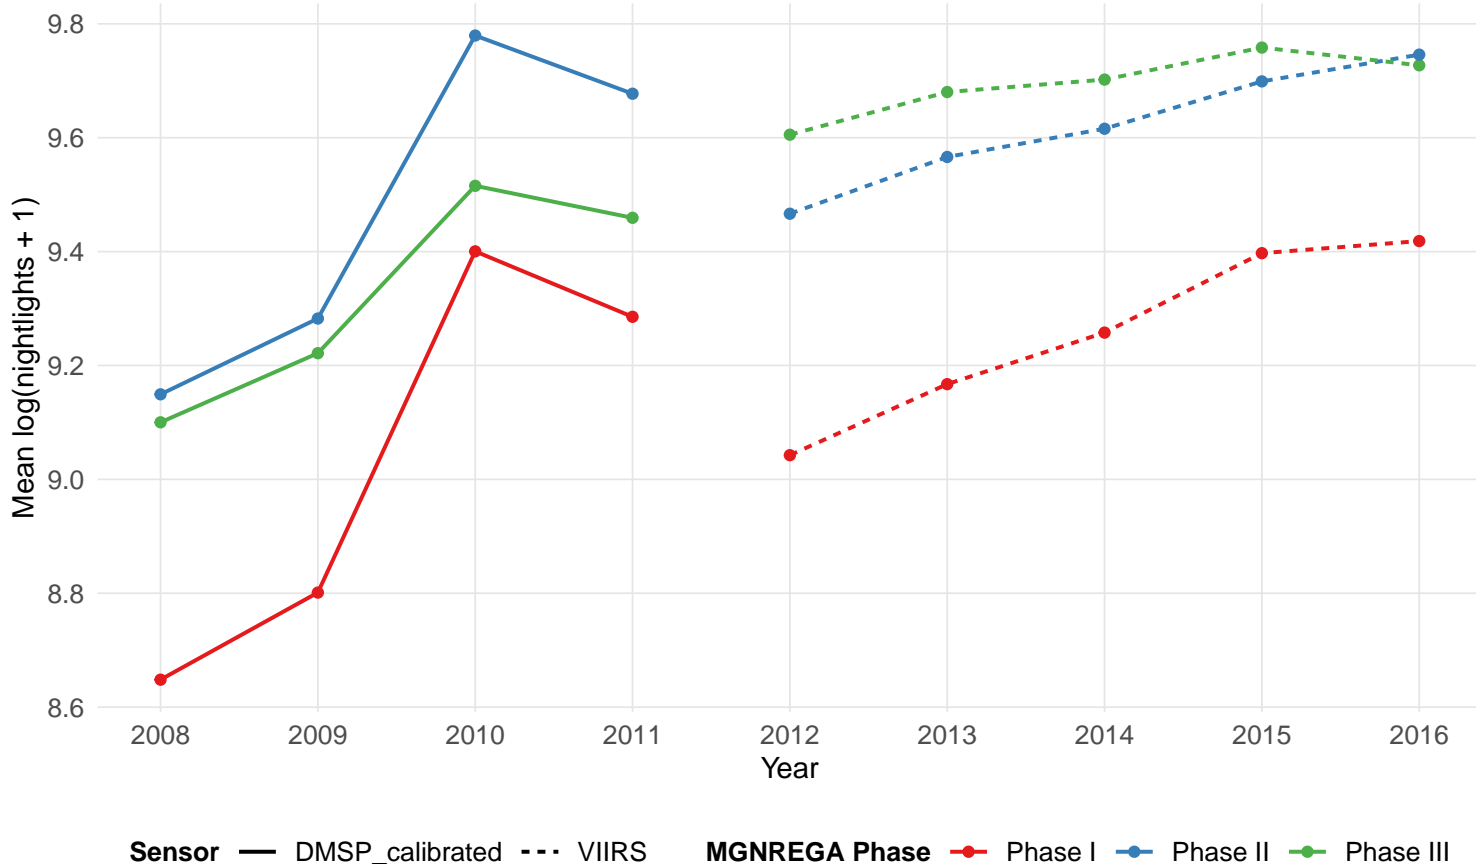

Note: DMSP (calibrated) and VIIRS overlap in 2012—2013.
Solid lines show the sensor used in the main analysis.