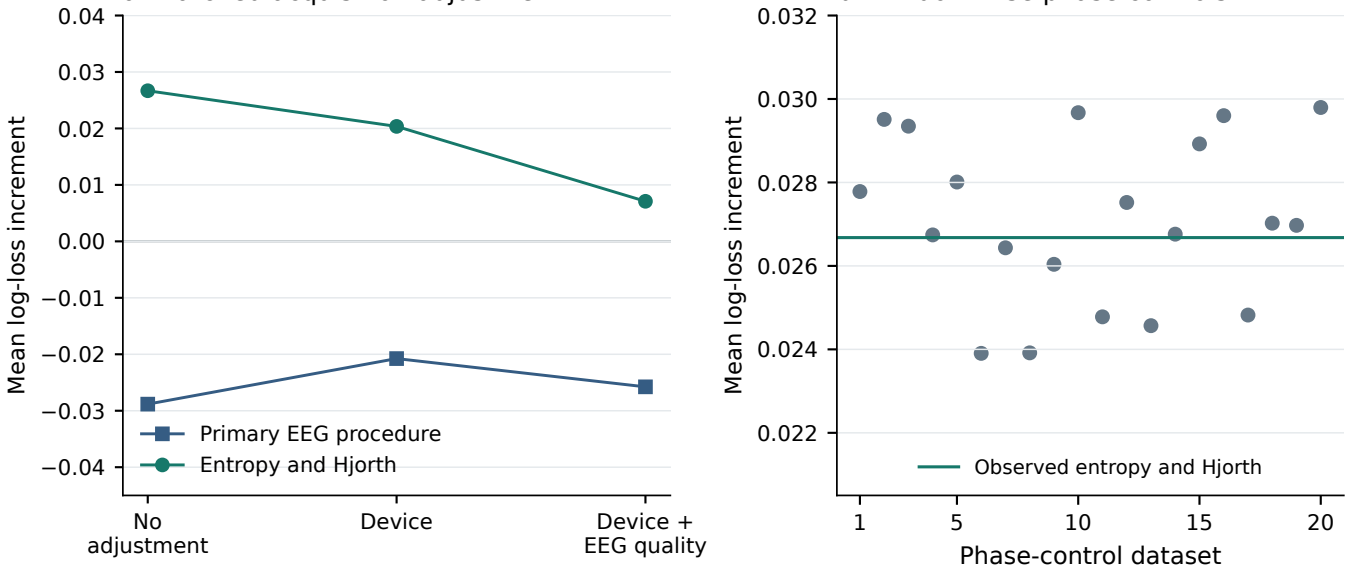
a Matched acquisition adjustment
Mean log-loss increment
0.04
0.03
0.02
0.01
0.00
−0.01
−0.02
−0.03
−0.04
Primary EEG procedure
Entropy and Hjorth
No adjustment
Device
Device + EEG quality
b Window-wise phase controls
Mean log-loss increment
0.032
0.030
0.028
0.026
0.024
0.022
Observed entropy and Hjorth
1
5
10
15
20
Phase-control dataset