



Individual samples in controlled T-cell PolyA/Ribo-sensitive directions


OSD-48 RR1

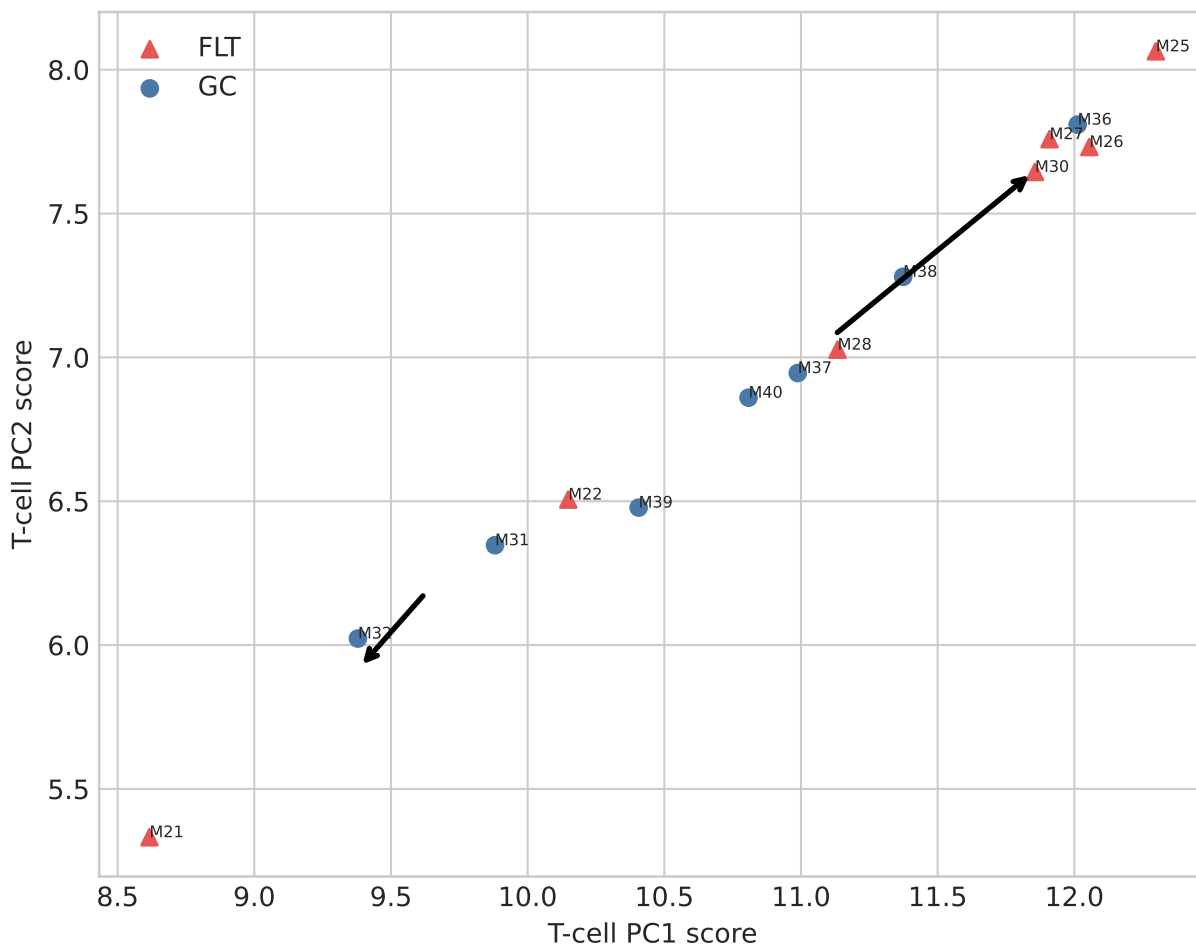

OSD-168 RR1

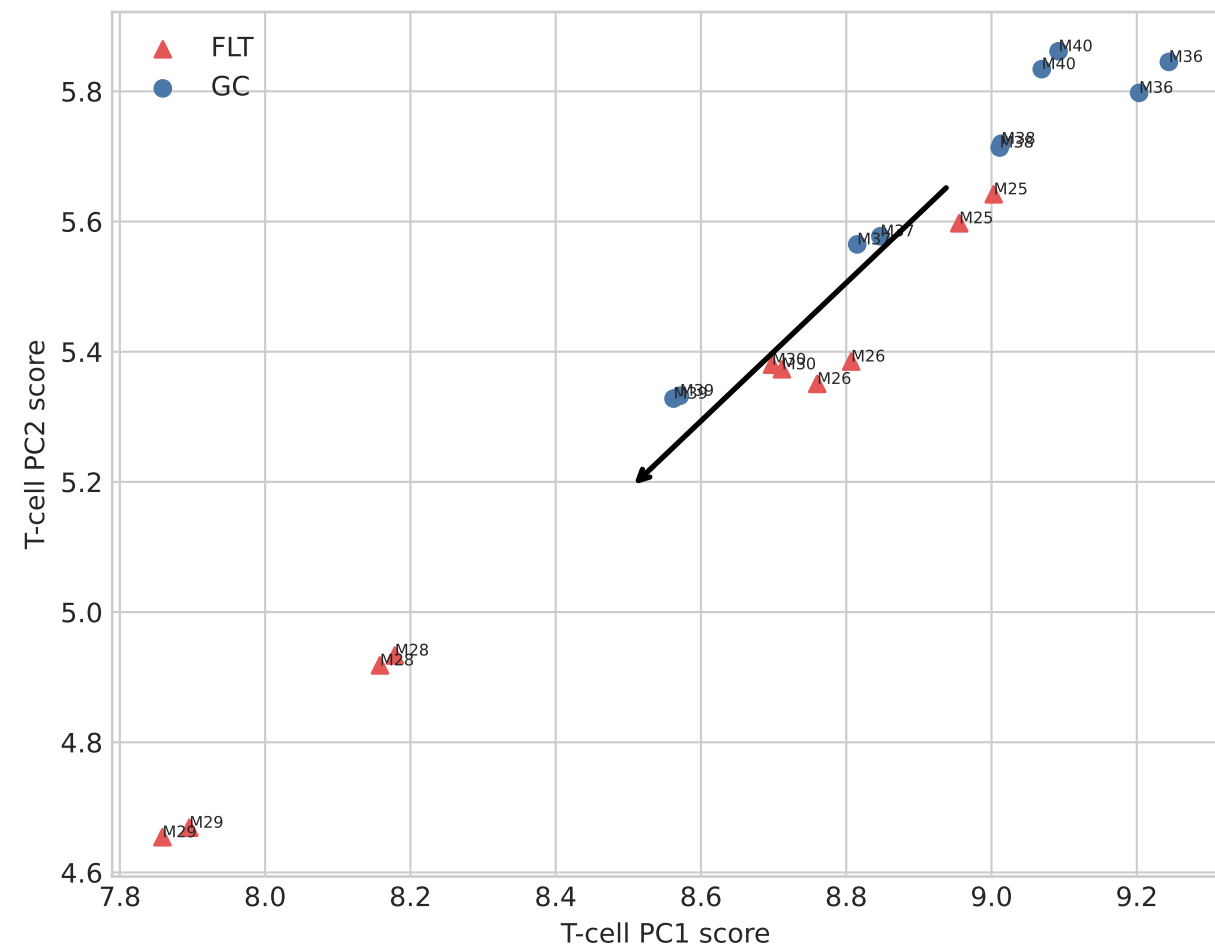

OSD-137 RR3

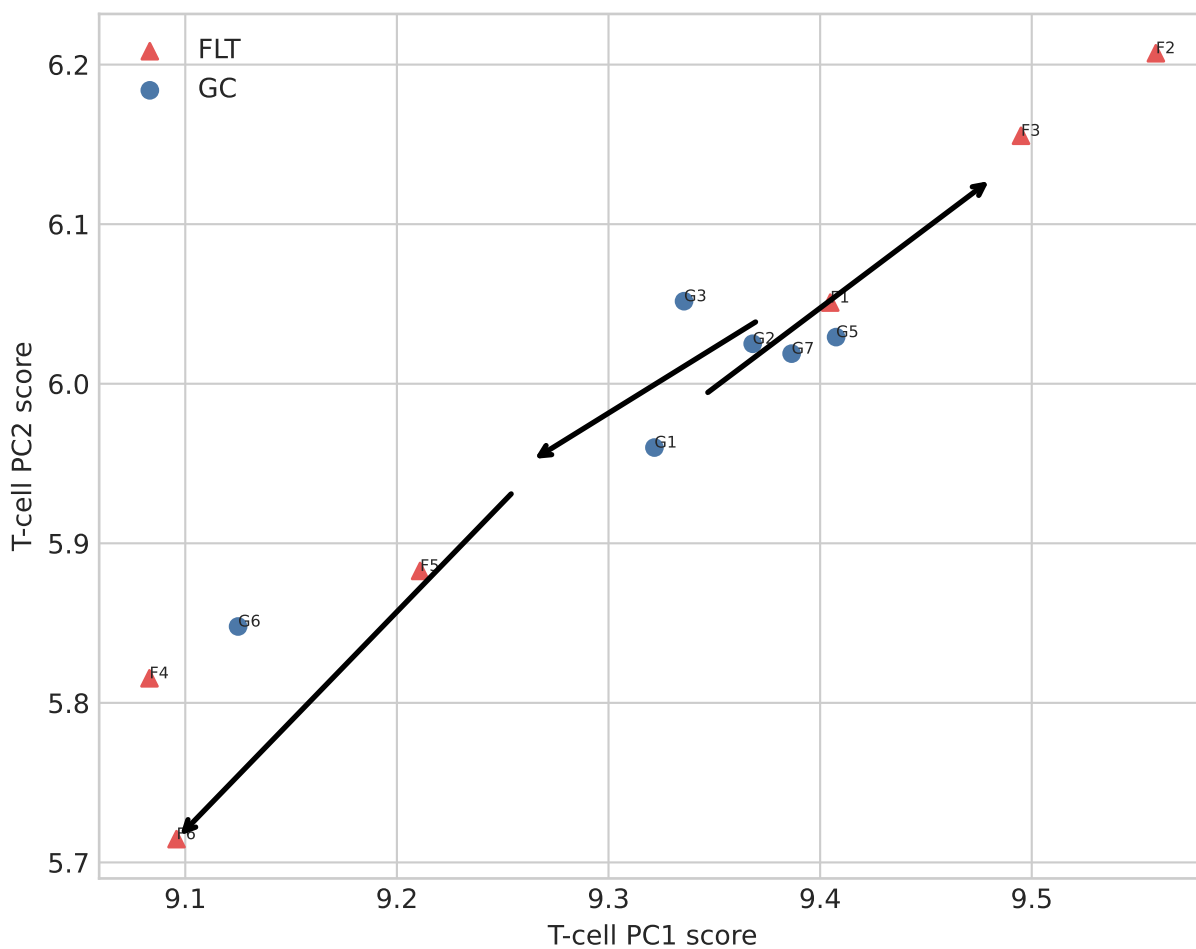

OSD-168 RR3

