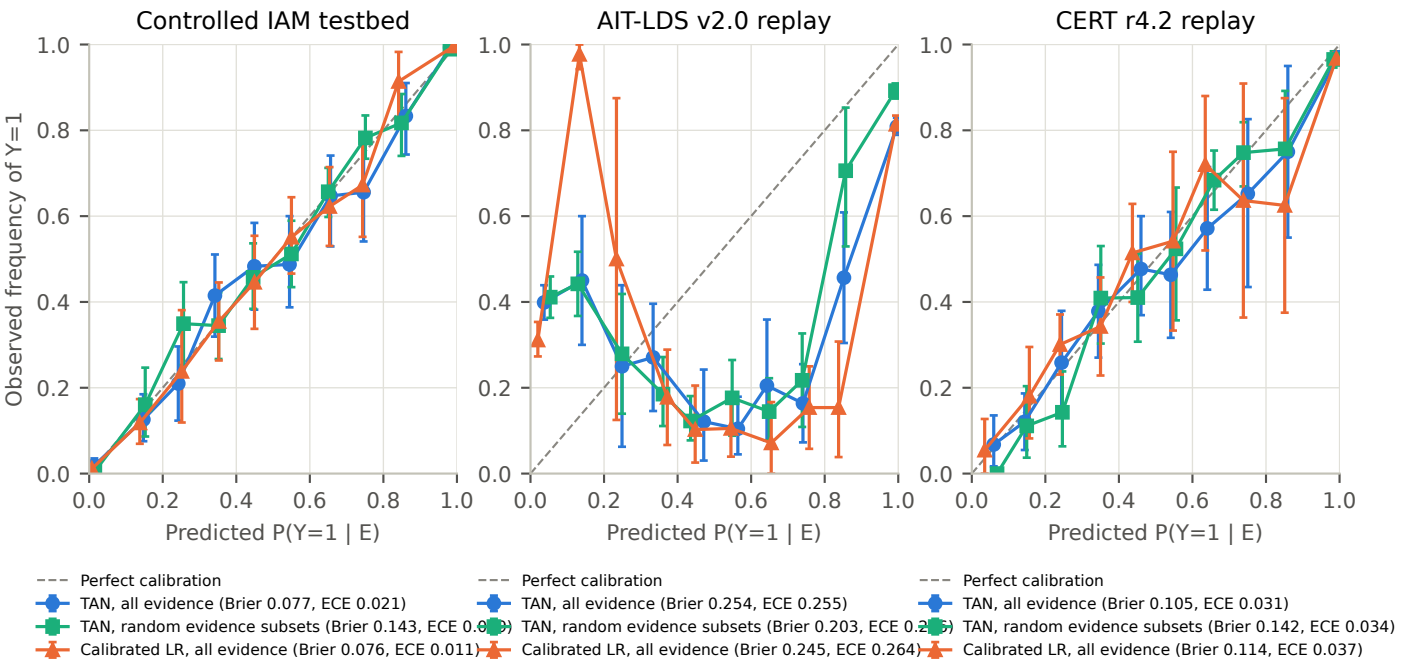
Calibration / reliability of the evidence models (held-out, 10 bins, 95% CI)
Controlled IAM testbed
AIT-LDS v2.0 replay
CERT r4.2 replay
Observed frequency of Y=1
Predicted P(Y=1 | E)
0.0
0.2
0.4
0.6
0.8
1.0
Perfect calibration
TAN, all evidence (Brier 0.077, ECE 0.021)
TAN, random evidence subsets (Brier 0.143, ECE 0.0
Calibrated LR, all evidence (Brier 0.076, ECE 0.011)
Perfect calibration
TAN, all evidence (Brier 0.254, ECE 0.255)
TAN, random evidence subsets (Brier 0.203, ECE 0.2
Calibrated LR, all evidence (Brier 0.245, ECE 0.264)
Perfect calibration
TAN, all evidence (Brier 0.105, ECE 0.031)
TAN, random evidence subsets (Brier 0.142, ECE 0.034)
Calibrated LR, all evidence (Brier 0.114, ECE 0.037)