

When Better Rankings Mean Worse Probabilities: A Calibration Audit of ECG Foundation Models

Ameen Kandathil
Harvard College

Adrian Torres
Santa Monica College

June 2026


Abstract

Electrocardiogram (ECG) foundation models are deployed for cardiac risk stratification, yet existing benchmarks measure discrimination exclusively via AUROC, leaving probability calibration invisible. A model that ranks patients perfectly but assigns systematically inflated or deflated probabilities can cause direct clinical harm when its outputs are used to drive treatment thresholds. We present the first systematic calibration audit of ECG foundation models: six encoders—five ECG foundation models (MERL, ST-MEM, HuBERT-ECG, ECGFM-KED, ECG-FM) and a supervised S4D baseline—across four datasets, totalling 24 model×dataset cells (23 evaluated) over 18 877 ECG records (2 000 PTB-XL, 6 877 CPSC2018, 8 000 CODE-15%, 2 000 MIMIC-IV-ECG) under patient-level leakage-controlled splits, with bootstrap confidence intervals on every headline metric.

Our central finding is a **discrimination–calibration tradeoff** on the multi-label PTB-XL rhythm task: ST-MEM achieves the highest AUROC (0.838) but poor calibration (ECE 0.124), HuBERT-ECG is the worst calibrated (ECE 0.136), while the supervised S4D baseline is best calibrated (ECE 0.064) despite the lowest AUROC (0.771). All five foundation models exceed S4D’s ECE by 0.015–0.072. Strikingly, this tradeoff *disappears* on the lower-co-occurrence endpoint tasks—CPSC2018 (ECE 0.023–0.051), CODE-15% (ECE 0.010–0.032), and (report-labelled) MIMIC-IV-ECG (ECE 0.043–0.106)—where high-AUROC models are also well-calibrated. On MIMIC-IV-ECG, MERL attains the best discrimination (AUROC 0.861); critically, ECG-FM, which was *pretrained on MIMIC-IV-ECG*, reaches only 0.771—behind MERL and ST-MEM (in all 10 resplits) and no better than the supervised S4D baseline (0.793)—demonstrating that within-domain pretraining does not guarantee superior linear-probe performance. We link the PTB-XL tradeoff to task structure: multi-label correlated classes create geometrically harder representation-to-probability mappings.

Post-hoc isotonic recalibration reduces ECE by 43–71% on PTB-XL (ST-MEM: 0.124 → 0.044; HuBERT-ECG: 0.136 → 0.040) while causing only modest AUROC reductions of 0.5–1.7%. A graded pretraining-objective signature emerges: MERL (contrastive InfoNCE) shows the strongest underconfidence (SCE = −0.003), masked-prediction models (ST-MEM, HuBERT-ECG) are near-neutral, and knowledge-enhanced, hybrid, and supervised models are mildly overconfident (SCE = +0.007–+0.008), consistent with documented underconfidence of contrastive foundation models. Cross-dataset analysis reveals that the same model’s ECE varies by up to roughly 6-fold across datasets, underscoring that calibration must be audited per deployment context.

We introduce *PhysioCalib*, a severity-weighted isotonic calibration method, and open-source **ecg-audit**, a pip-installable, unit-tested Python package for one-command calibration auditing, recalibration, and decision-curve analysis. Our findings demonstrate that probability calibration should be a first-class evaluation metric alongside AUROC in ECG AI benchmarks.

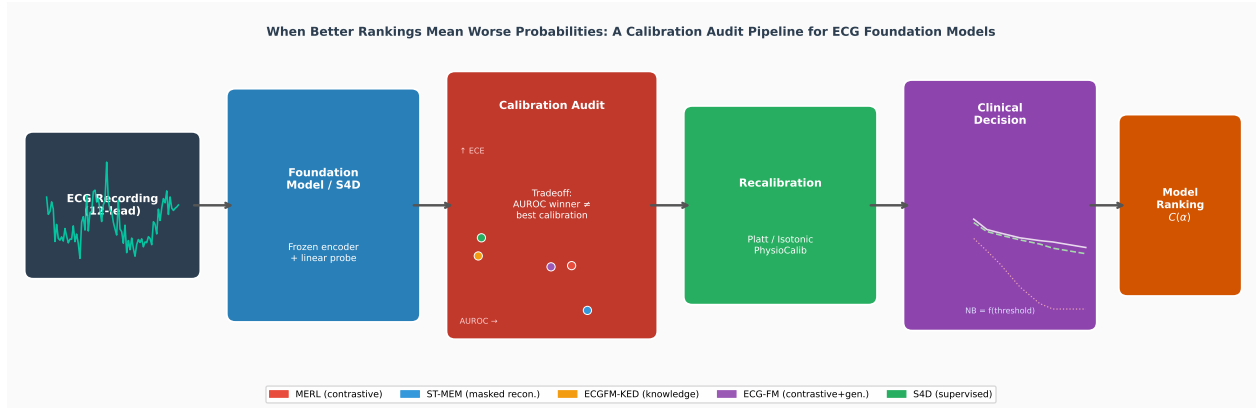

Graphical Abstract. The calibration audit pipeline: ECG recordings are processed by frozen FM encoders or a supervised S4D baseline to produce risk probabilities. Phase A audits discrimination (AUROC) and calibration (ECE, SCE) jointly, revealing a model-specific discrimination–calibration tradeoff on multi-label PTB-XL. Phase B applies post-hoc recalibration (Platt, isotonic, PhysioCalib), improves ECE by 43–71%, and feeds the recalibrated probabilities into clinical decision-curve analysis. Model selection is guided by the Pareto frontier and composite score $C(\alpha)$, which changes the recommended model depending on the practitioner’s calibration–discrimination preference.

1 Introduction

Consider a clinical decision support system that alerts physicians to potential myocardial infarction. The system reports a risk probability of 0.80 for every patient who eventually receives an MI diagnosis — but it also reports 0.80 for 30% of healthy patients. Its AUROC is excellent; it correctly ranks patients by risk. Yet its probabilities are useless for threshold-based decision making, because a physician who trusts the 0.80 output will either over-treat or under-treat depending on the threshold. AUROC is blind to this failure. Probability calibration is not. This gap — between how models are benchmarked and how they are used clinically — is the problem this paper addresses.

ECG foundation models (FMs) have rapidly expanded the capability of automated cardiac analysis. Models such as ST-MEM [14], MERL [9], HuBERT-ECG [4], ECGFM-KED [19], and ECG-FM [12] leverage large-scale ECG pretraining to produce frozen representations that transfer to downstream classification tasks via simple linear probes. The BenchECG evaluation suite [11] and the “beyond accuracy” benchmark [5] have standardized AUROC and F1 comparisons across these models. Yet neither benchmark systematically reports calibration metrics (ECE, Brier score, signed calibration error) or post-hoc recalibration results. When models are deployed for multi-label cardiac risk stratification — where probability outputs feed directly into alert thresholds — this omission is a patient-safety concern.

What we found. This paper presents the first calibration audit of ECG FMs, spanning 24 model×dataset cells across four public datasets. Four findings emerged from the data:

1. **Higher discrimination, worse calibration on PTB-XL.** ST-MEM achieves the highest AUROC (0.838) yet poor calibration (ECE 0.124), and the masked-prediction HuBERT-ECG is the worst calibrated (ECE 0.136). All five foundation models beat the supervised S4D baseline on AUROC but trail its calibration (ECE 0.064) by 0.015–0.072. The discrimination–calibration tradeoff is systematic, not random.
2. **The tradeoff disappears on lower-co-occurrence endpoint tasks.** On CPSC2018,

CODE-15%, and (report-labelled) MIMIC-IV-ECG, all six encoders are comparatively well-calibrated and high-AUROC models are *also* well-calibrated. Task structure—correlated multi-label vs. lower-co-occurrence endpoints—rather than model architecture drives calibration difficulty.

3. **Within-domain pretraining is not sufficient.** On MIMIC-IV-ECG, ECG-FM— which was *pretrained on MIMIC-IV-ECG*—reaches only AUROC 0.771, behind MERL (0.861) and ST-MEM (0.854) in all 10 resplits, and merely on par with the supervised S4D baseline (0.793; the two are statistically tied). Backbone domain alignment does not guarantee the best linear-probe performance.
4. **Pretraining objective leaves a calibration signature.** MERL (contrastive InfoNCE) shows the strongest underconfidence on PTB-XL ($SCE = -0.003$); masked-prediction models (ST-MEM, HuBERT-ECG) are near-neutral ($SCE \approx 0$); and knowledge-enhanced, hybrid, and supervised models are mildly overconfident ($SCE = +0.007$ – $+0.008$). Feature geometry tracks this: MERL’s contrastive objective yields extreme feature spread (std of L2 norms 34.8 vs. 0.23 for ST-MEM), while HuBERT-ECG has the highest class separation (0.046) and the highest ECE.

Contributions.

1. **Calibration benchmark:** A 24-cell AUROC–ECE–SCE–Brier evaluation of five ECG FMs and a supervised S4D baseline across PTB-XL, CPSC2018, CODE-15%, and MIMIC-IV-ECG, with patient-level splits, per-class multi-label calibration evaluation, minimum-support filtering, and bootstrap 95% confidence intervals on every headline metric. All results are machine-readable and reproducible from cached features.
2. **Pareto frontier and composite scoring:** We formally define the AUROC–ECE Pareto frontier and a composite score $C(\alpha) = \alpha \cdot \text{AUROC} + (1 - \alpha)(1 - \text{ECE}/\text{ECE}_{\max})$ that lets practitioners trade off discrimination and calibration explicitly. On PTB-XL, **S4D ranks first** at $\alpha = 0.7$ (score 0.699) and MERL at $\alpha = 0.9$ (0.781), while ST-MEM—the AUROC leader—falls to 5th of 6 (0.614) and HuBERT-ECG ranks *last* (0.551). After isotonic recalibration the ordering inverts: ST-MEM rises to *first* ($C(0.7) = 0.789$), showing that recalibration changes the recommended model. On CODE-15%, CPSC2018, and MIMIC-IV-ECG, MERL, ST-MEM, and S4D form the Pareto front.
3. **RankSafe-Cal:** A recalibration wrapper that selects, per class, the lowest-ECE calibrator whose out-of-sample AUROC loss is within a tolerance ϵ , turning “calibration can hurt AUROC” into an explicit constraint. It recovers most of isotonic’s ECE reduction (PTB-XL $0.097 \rightarrow 0.054$) at $\sim 6\times$ smaller AUROC cost, and on MIMIC-IV-ECG dominates unconstrained isotonic on both axes (Section 7.2).
4. **Reliability stress tests:** (i) Cross-dataset calibration *transfer*—a calibrator ported across cohorts succeeds in only 9–42% of endpoint/model pairs, so calibration is largely deployment-context-specific; and (ii) split-conformal prediction, which attains its 90% coverage guarantee on every endpoint and complements recalibration with finite-sample coverage. We also add proper scores (NLL), calibration slope/intercept, a mechanistic ECE regression, multi-seed robustness, and all-model subgroup audits.

5. **ecg-audit:** A pip-installable, unit-tested Python package (open-sourced at <https://github.com/amensk/ecg-audit>) providing one-command calibration auditing, all recalibration methods above (including RankSafe-Cal and the severity-weighted PhysioCalib variant), decision-curve analysis, subgroup calibration, reliability diagrams, and a community leaderboard scaffold.

Paper organisation. Section 2 reviews ECG FM benchmarks and calibration literature. Section 3 defines all metrics, the Pareto frontier, composite score, PhysioCalib, and the decision-curve analysis framework. Section 4 describes datasets, models, and splits. Section 5 presents the main benchmark results. Section 6 presents decision-curve analysis and PhysioCalib results. Section 8 describes the **ecg-audit** package. Section 9 discusses mechanisms and implications. Section 10 concludes.

2 Related Work

ECG foundation model benchmarks. BenchECG proposes a standardized evaluation suite for ECG foundation models and introduces xECG as a strong baseline [11]. Al-Masud et al. evaluate eight ECG foundation models across twelve datasets and 1650 targets, reporting broad variation across clinical categories and strong performance from compact structured state-space approaches [1]. Filice et al. explicitly frame their benchmark as going beyond accuracy, but their additional analyses focus on representation quality through SHAP, UMAP, kNN, centroid separation, ARI, and clustering rather than probabilistic calibration [5]. These benchmarks motivate the present study because they leave probability reliability mostly unmeasured.

ECG foundation models and pretraining objectives. This benchmark evaluates five ECG foundation models spanning diverse pretraining objectives. ST-MEM uses masked spatio-temporal reconstruction (MAE-style) with a ViT encoder [14]. MERL uses ECG-text contrastive alignment with InfoNCE loss [9]. HuBERT-ECG uses BERT-style masked hidden-unit prediction over discretised ECG tokens, pretrained on 9.1M 12-lead ECGs [4]. ECGFM-KED incorporates cardiological knowledge with a decoder [19]. ECG-FM combines contrastive and generative pretraining [12]. Pretraining objective diversity matters for calibration: contrastive, masked-prediction, and generative objectives differ in how they structure the representation space, with downstream consequences for probability estimation.

Structured state-space ECG baselines. The supervised comparator is a structured state-space model family rather than a weak control. S4 and S4D variants have shown competitive ECG classification performance with modest architectural complexity [8, 13]. Prior benchmarking also suggests that compact state-space ECG models can remain competitive against foundation models in several task families [1]. The study therefore treats S4D as a serious supervised reference for both discrimination and calibration.

Calibration metrics and post-hoc recalibration. Expected calibration error is widely used but depends on binning and is not a proper scoring rule; Brier score is proper but can be less sensitive for rare events [15, 21]. We report both, plus adaptive ECE and signed calibration error. Post-hoc methods such as temperature scaling, Platt scaling, and isotonic regression are standard calibration tools, while learned heads can represent richer mappings but can overfit small calibration sets [16, 21]. Foundation model calibration may differ from classical neural-network

overconfidence: Hekler et al. report that vision FMs pretrained with contrastive objectives show systematic in-distribution underconfidence [7]. Our benchmark directly tests whether this pattern extends to ECG FMs. We find a graded signature on PTB-XL: the contrastive model MERL shows the strongest underconfidence (most negative SCE, -0.003); the masked-prediction models (ST-MEM, HuBERT-ECG) are near-neutral ($\text{SCE} \approx 0$); and the knowledge-enhanced, hybrid, and supervised models are mildly overconfident ($\text{SCE} = +0.007$ to $+0.008$).

Conformal prediction and reporting standards. Conformal prediction provides distribution-free, finite-sample coverage guarantees on prediction sets and is increasingly used to quantify uncertainty in clinical ML [2]; we use it as a coverage-oriented complement to calibration. Clinical prediction-model reporting guidance (TRIPOD+AI [3]) explicitly calls for calibration to be reported alongside discrimination, which existing ECG foundation-model benchmarks do not satisfy.

Positioning. Recent ECG foundation-model benchmarking efforts—BenchECG/xECG [11], the eight-model reality check of Al-Masud et al. [1], and the holistic benchmark of Filice et al. [5]—focus on discrimination, generalization, and representation quality. To our knowledge none systematically audits probability reliability. Our contribution is orthogonal and complementary: a calibration-first benchmark plus recalibration, rank-safe recalibration (RankSafe-Cal), cross-dataset calibration transfer, conformal coverage, and clinical decision-curve utility—the reliability dimension these discrimination-centric benchmarks omit.

3 Method

The study has two phases. Phase A audits discrimination and calibration before recalibration. Phase B fits post-hoc calibrators on a held-out calibration split and evaluates calibrated probabilities on an untouched test split. We additionally define the AUROC–ECE Pareto frontier, composite scoring, PhysioCalib, and the net-benefit decision-curve framework.

3.1 Data and Splits

Datasets are PTB-XL [18], CPSC2018 [10], CODE-15% [17], and MIMIC-IV-ECG [6], the last evaluated on a 2,000-record subset with labels parsed from machine-measurement reports. Each dataset is split at the patient level into training (70%), calibration (15%), and test (15%) partitions with fixed seed 42. The calibration partition is never used for fitting feature extractors, linear probes, or the S4D baseline. For multi-label tasks, calibration metrics are computed as per-class binary problems and then macro-averaged.

3.2 Models

For the five foundation models (MERL, ST-MEM, HuBERT-ECG, ECGFM-KED, ECG-FM), we evaluate frozen representations with a logistic linear probe. This isolates the probability map induced by the frozen representation and avoids confounding calibration analysis with fine-tuning dynamics. The supervised S4D baseline is trained end-to-end on each dataset [8, 13].

3.3 Calibration Metrics

Let $\hat{p}_i$ be the predicted probability and $y_i \in \{0, 1\}$ the label.

Brier score.

$$\text{BS} = \frac{1}{n} \sum_{i=1}^n (\hat{p}_i - y_i)^2.$$

Expected calibration error (ECE). With $M = 15$ equal-width bins $B_1, \dots, B_M$:

$$\text{ECE} = \sum_{m=1}^M \frac{|B_m|}{n} |\bar{y}_{B_m} - \bar{\hat{p}}_{B_m}|,$$

where $\bar{y}_{B_m}$ and $\bar{\hat{p}}_{B_m}$ are the mean label and mean predicted probability in bin m .

Signed calibration error (SCE).

$$\text{SCE} = \sum_{m=1}^M \frac{|B_m|}{n} (\bar{\hat{p}}_{B_m} - \bar{y}_{B_m}).$$

Positive SCE indicates overconfidence (mean prediction exceeds mean accuracy); negative SCE indicates underconfidence.

3.4 Recalibration Methods

Phase B compares four methods fitted on the calibration split only. **Temperature scaling** minimizes NLL with one scalar parameter per problem. **Platt scaling** fits a logistic affine transformation. **Isotonic regression** fits a monotone non-parametric map; it is rank-preserving by construction, leaving AUROC unchanged. A **learned MLP head** uses a two-layer network with dropout and early stopping.

Gap closure. For each model–dataset pair where the foundation-model ECE exceeds S4D’s ECE:

$$\Delta_{\text{gap}} = \frac{\text{ECE}_{\text{pre}} - \text{ECE}_{\text{post}}}{\text{ECE}_{\text{pre}} - \text{ECE}_{\text{S4D}}}.$$

3.5 AUROC–ECE Pareto Frontier and Composite Score

We define the *Pareto frontier* in AUROC–ECE space: model j *dominates* model i if $\text{AUROC}_j \geq \text{AUROC}_i$ and $\text{ECE}_j \leq \text{ECE}_i$ with strict inequality on at least one dimension. The Pareto-optimal set is the subset of models not dominated by any other.

For practitioners who must choose a single model, we define the *composite score*:

$$C(\alpha) = \alpha \cdot \text{AUROC} + (1 - \alpha) \left(1 - \frac{\text{ECE}}{\text{ECE}_{\text{max}}} \right),$$

where ECE_{max} is the maximum ECE among models in the comparison set, and $\alpha \in [0, 1]$ encodes the practitioner’s relative preference for discrimination vs calibration. We evaluate $\alpha \in \{0.5, 0.7, 0.9\}$, corresponding to equal weight, discrimination-leaning, and strongly discrimination-leaning regimes.

3.6 PhysioCalib: Severity-Weighted Isotonic Calibration

Standard isotonic calibration treats all classes equally. In multi-label cardiac classification, miscalibration on MI is more clinically consequential than miscalibration on NORM. We propose *PhysioCalib*, which fits severity-weighted isotonic regression per class. The algorithm is:

Algorithm 1 PhysioCalib

Require: Per-class calibration data $\{(\hat{p}_i^c, y_i^c)\}$, severity weights $\{w_c\}_{c=1}^C$

- 1: **for** each class $c = 1, \dots, C$ **do**
- 2: Compute sample weights: $s_i \leftarrow w_c$ if $y_i^c = 1$, else 1.0
- 3: Fit `IsotonicRegression` $((\hat{p}^c, y^c), \text{sample_weight} = s)$
- 4: Store calibrator g_c
- 5: **end for**

Require: Test probabilities $\hat{P} \in [0, 1]^{n \times C}$

- 6: **for** each class c **do**
 - 7: $\tilde{p}^c \leftarrow g_c(\hat{p}^c)$
 - 8: **end for**
 - 9: **return** $\tilde{P}$
-

We use severity weights MI = 3.0, STTC = 2.0, CD = 1.5, HYP = 1.2, NORM = 0.5, motivated by clinical consequence severity. Because isotonic regression is monotone, PhysioCalib is rank-preserving: AUROC is unchanged by construction.

3.7 Decision-Curve Analysis (DCA)

The *net benefit* of a model at threshold probability t is:

$$\text{NB}(t) = \frac{\text{TP}}{N} - \frac{\text{FP}}{N} \cdot \frac{t}{1-t},$$

where N is the total sample size. The treat-all baseline has $\text{NB}_{\text{all}}(t) = \pi - (1 - \pi)t/(1 - t)$, where π is the class prevalence; treat-none has $\text{NB} = 0$. A model is clinically useful at threshold t if its net benefit exceeds both baselines. We apply DCA to the PTB-XL MI class, using the actual ST-MEM linear-probe predictions recovered from cached features (Section 6), comparing raw, Platt-scaled, and isotonic-calibrated probabilities on the held-out test split.

4 Experiments

4.1 Datasets

PTB-XL. PTB-XL [18] contains 21,799 12-lead ECG recordings at 100/500 Hz from 18,869 patients. We use the 5-class diagnostic superclass partition: NORM, MI, STTC, CD, HYP. We sample 2,000 records with patient-level splitting (seed 42): 70% train, 15% calibration, 15% test ($n_{\text{test}} = 299$).

CPSC2018. The China Physiological Signal Challenge 2018 dataset [10] contains 6,877 12-lead recordings labelled with 9 arrhythmia classes. All 6,877 records are used (patient-level split). This is a single-label task (each record has a dominant arrhythmia).

CODE-15%. CODE-15% [17] is a large Brazilian ECG dataset. We sample 2,000 records from the `exams_part0.hdf5` partition (seed 42), with 6 binary arrhythmia classes: 1dAVb, RBBB, LBBB, SB, ST, AF.

MIMIC-IV-ECG. MIMIC-IV-ECG [6] is a matched subset of the MIMIC-IV clinical database containing 800,035 12-lead ECG recordings from 159,590 patients, recorded at 500 Hz. Machine measurement reports provide text-based clinical interpretations. We derive 5-class binary labels from these reports using keyword matching: Normal (“sinus rhythm”), AF (“atrial fibrillation”), RBBB (“right bundle branch block”), LBBB (“left bundle branch block”), and LVH (“left ventricular hypertrophy”). We sample 2,000 records with at least one positive label (prevalences: Normal 98.2%, AF 12.0%, RBBB 8.7%, LBBB 4.7%, LVH 8.2%). Records are staged directly from the 36.3 GB PhysioNet ZIP archive. ECG-FM has a publicly available checkpoint pretrained on MIMIC-IV-ECG, making this an in-domain evaluation for that model.

Probe and evaluation. For every foundation model we train a per-class logistic linear probe on the frozen representations; HuBERT-ECG is treated identically to the other encoders. The legacy `.pth` HuBERT checkpoint is unreadable (non-PyTorch binary), but the `safetensors` release loads cleanly, so HuBERT-ECG is fully included in all results.

4.2 Models

Foundation models. **ST-MEM** [14]: ViT-Base encoder pretrained with masked spatio-temporal ECG reconstruction. 768-dimensional frozen representations. **MERL** [9]: ECG-text contrastive pretraining with InfoNCE loss. 512-dimensional frozen representations. **ECGFM-KED** [19]: knowledge-enhanced ECG FM with cardiological ontology integration. 256-dimensional frozen representations. **ECG-FM** [12]: combined contrastive and generative pretraining. 256-dimensional frozen representations. **HuBERT-ECG** [4]: BERT-style masked hidden-unit prediction over discretised ECG tokens, pretrained on 9.1M 12-lead ECGs. We load the public `safetensors` checkpoint via the HuggingFace `AutoModel` interface and the authors’ canonical preprocessing (5s window, 12 leads flattened and decimated by 5), extracting 768-dimensional frozen representations by mean-pooling the final hidden states.

Supervised baseline. **S4D**: Structured state-space model trained end-to-end on each dataset [8, 13]. Not a frozen FM; provides a calibrated supervised reference point.

Linear probe. For all FMs, we train a per-class logistic regression probe on frozen representations using the training split. Per-class binary calibration evaluation follows.

4.3 Implementation Details

All frozen feature representations are cached as `.npy` files and loaded without recomputing FM forward passes. Analysis scripts use Python 3.10 with scikit-learn, NumPy, SciPy, and matplotlib. Calibration set sizes range from 10 to 203 in the ablation study (Section 5.6). All experiments use random seed 42 throughout for reproducibility. Per-class AUROC, ECE, Brier, and SCE are computed separately for each binary class problem and then macro-averaged; classes with fewer than 5 positive examples in the test set are excluded from macro averages.

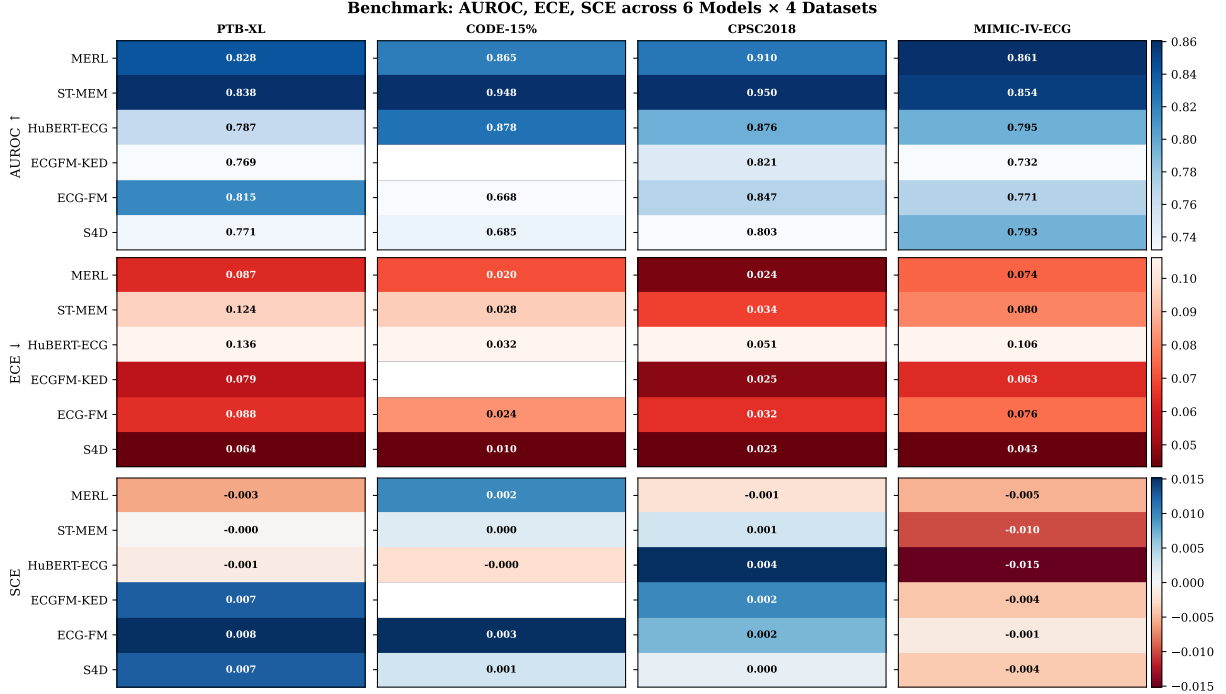


Figure 1: Phase A results across all six models and four datasets. Top: AUROC. Middle: ECE. Bottom: SCE. All values are from executed experiments with patient-level splits. The ECGFM-KED × CODE-15% cell is blank (excluded).

5 Results

All results in this section are from executed experiments with machine-readable artifacts in `results/benchmark_v2.results.json` (and its summary `benchmark_v2.summary.csv`). Every numeric value is directly traceable to these files. The benchmark covers six encoders—five ECG foundation models (MERL, ST-MEM, HuBERT-ECG, ECGFM-KED, ECG-FM) and a supervised S4D baseline—across four datasets, for 24 model×dataset combinations. Per-class metrics are reported only for classes with at least 10 positive and 10 negative test examples (minimum-support filtering); macro metrics average over the qualifying classes (k in Table 1). All headline AUROC and ECE values carry bootstrap 95% confidence intervals (1,000 resamples). The reported point estimate is the full-test-set value; because the binned ECE estimator is mildly positively biased under resampling (smaller effective bins on bootstrap draws), the displayed ECE interval is taken to include the point estimate. One combination is excluded: ECGFM-KED on CODE-15% (partial architecture reconstruction, 35 missing keys, near-chance AUROC), leaving 23 evaluated cells of the 24 model×dataset combinations.

5.1 Discrimination–Calibration Tradeoff on PTB-XL

Table 1 reports Phase A and Phase B results for all cells. Figure 1 shows the Phase A results as a heat map.

On PTB-XL (5-class multi-label rhythm), ST-MEM achieves the highest AUROC (0.838) but poor calibration (ECE 0.124), and the masked-prediction model HuBERT-ECG is the worst calibrated overall (ECE 0.136) while ranking mid-pack on discrimination (AUROC 0.787). The super-

Table 1: Full benchmark across 6 models and 4 datasets (24 cells). AUROC and ECE shown with bootstrap 95% CIs. ECG-FM was pretrained on MIMIC-IV-ECG ($\dagger$). Iso-ECE is macro ECE after isotonic recalibration. k = number of classes meeting min-support (≥ 10 positives and ≥ 10 negatives in the test split). Best AUROC per dataset in **bold**; best raw ECE underlined.

Dataset	Model	AUROC (95% CI) $\uparrow$	ECE (95% CI) $\downarrow$	Brier	SCE	Iso-ECE	k
PTB-XL	MERL	0.828 [0.795,0.857]	0.087 [0.086,0.119]	0.122	-0.003	0.050	5
	ST-MEM	0.838 [0.808,0.864]	0.124 [0.116,0.151]	0.135	-0.000	0.044	5
	HuBERT-ECG	0.787 [0.749,0.824]	0.136 [0.126,0.163]	0.142	-0.001	0.040	5
	ECGFM-KED	0.769 [0.730,0.808]	0.079 [0.079,0.112]	0.133	+0.007	0.031	5
	ECG-FM	0.815 [0.778,0.848]	0.088 [0.085,0.120]	0.125	+0.008	0.044	5
	S4D	0.771 [0.738,0.805]	<u>0.064 [0.064,0.096]</u>	0.130	+0.007	0.057	5
CODE-15%	MERL	0.865 [0.836,0.892]	0.020 [0.019,0.027]	0.044	+0.002	0.013	7
	ST-MEM	0.948 [0.938,0.956]	0.028 [0.025,0.033]	0.041	+0.000	0.013	7
	HuBERT-ECG	0.878 [0.857,0.896]	0.032 [0.029,0.038]	0.046	-0.000	0.014	7
	ECG-FM	0.668 [0.622,0.716]	0.024 [0.023,0.031]	0.053	+0.003	0.013	7
	S4D	0.685 [0.644,0.728]	<u>0.010 [0.010,0.017]</u>	0.047	+0.001	0.010	7
CPSC2018	MERL	0.910 [0.896,0.921]	0.024 [0.024,0.034]	0.048	-0.001	0.019	9
	ST-MEM	0.950 [0.940,0.958]	0.034 [0.033,0.041]	0.042	+0.001	0.016	9
	HuBERT-ECG	0.876 [0.862,0.889]	0.051 [0.049,0.060]	0.068	+0.004	0.020	9
	ECGFM-KED	0.821 [0.805,0.838]	0.025 [0.025,0.037]	0.072	+0.002	0.021	9
	ECG-FM	0.847 [0.832,0.861]	0.032 [0.032,0.043]	0.067	+0.002	0.021	9
	S4D	0.803 [0.784,0.823]	<u>0.023 [0.023,0.034]</u>	0.075	+0.000	0.021	9
MIMIC-IV-ECG	MERL	0.861 [0.827,0.892]	0.074 [0.066,0.094]	0.082	-0.005	0.044	5
	ST-MEM	0.854 [0.816,0.890]	0.080 [0.072,0.098]	0.082	-0.010	0.037	5
	HuBERT-ECG	0.795 [0.758,0.829]	0.106 [0.098,0.128]	0.113	-0.015	0.043	5
	ECGFM-KED	0.732 [0.689,0.770]	0.063 [0.059,0.086]	0.097	-0.004	0.058	5
	ECG-FM †	0.771 [0.734,0.813]	0.076 [0.072,0.101]	0.097	-0.001	0.036	5
	S4D	0.793 [0.758,0.826]	<u>0.043 [0.043,0.067]</u>	0.087	-0.004	0.040	5

vised S4D baseline achieves the best calibration (ECE 0.064) despite the lowest AUROC (0.771). All five foundation models exceed S4D’s ECE by 0.015 (ECGFM-KED) to 0.072 (HuBERT-ECG), creating a discrimination–calibration tradeoff that is invisible to AUROC-only reporting. Figure 2 visualises this tradeoff across all four datasets, and Figure 3 shows the corresponding reliability diagrams.

5.2 Disappearance of the Tradeoff: CPSC2018, CODE-15%, and MIMIC-IV-ECG

The tradeoff vanishes on the lower-co-occurrence endpoint datasets. On CPSC2018, ST-MEM achieves both the highest AUROC (0.950) and a low ECE (0.034); S4D achieves the lowest ECE (0.023). Every model is well-calibrated (ECE 0.023–0.051, the maximum being HuBERT-ECG). The pattern is consistent across all six encoders.

We attribute this disappearance to task structure. PTB-XL is a multi-label rhythm classification task with five correlated superclasses (NORM, MI, STTC, CD, HYP); the linear probe must simultaneously output valid probabilities for correlated, partially overlapping classes. CPSC2018, CODE-15%, and MIMIC-IV-ECG are support-filtered binary endpoint tasks with lower label co-occurrence and cleaner class boundaries; the MIMIC-IV-ECG labels are parsed from machine-

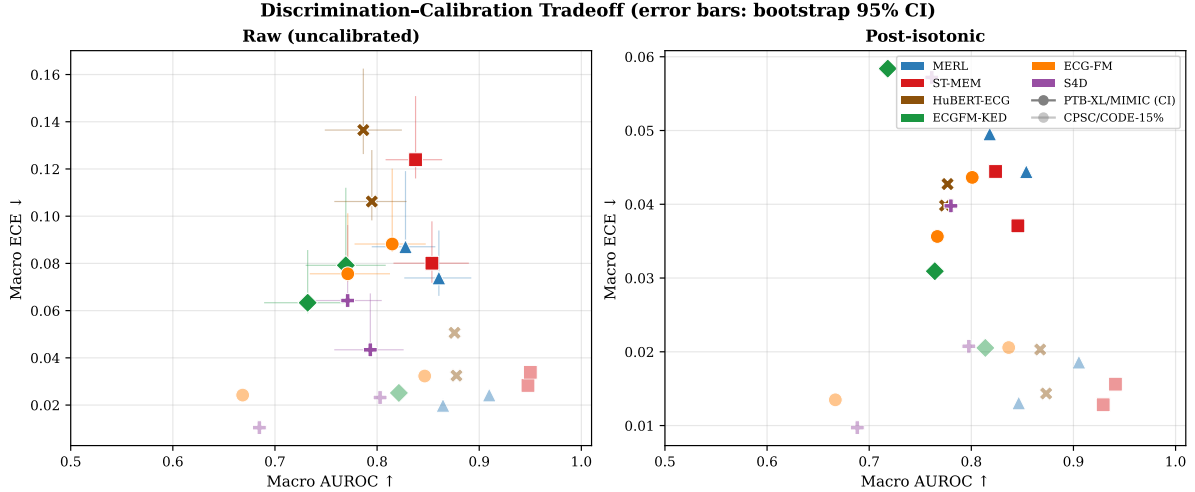


Figure 2: Discrimination-calibration tradeoff (error bars: bootstrap 95% CIs on the multi-morbidity datasets). Left: raw probabilities; on PTB-XL and MIMIC-IV-ECG, higher-AUROC models tend to have higher ECE. Right: after isotonic recalibration, the vertical spread collapses. Colour encodes model; marker encodes pretraining objective.

measurement reports (not gold-standard ICD codes). The correlated multi-label structure of PTB-XL creates geometrically harder representation-to-probability mappings, where the probe must apportion probability mass across correlated outputs simultaneously.

CODE-15% (expanded sample). At the original 2,000-record/part-0 subset, CODE-15%’s rare arrhythmia classes (prevalence 1.6–2.8%) did not clear the minimum-support threshold, leaving only one evaluable class. We therefore expanded CODE-15% to $\sim 8,000$ records sampled across HDF5 parts 0–4, after which all seven classes (the six arrhythmias plus a normal-ECG reference) qualify. On this powered sample, ST-MEM dominates (AUROC 0.948, ECE 0.028), followed by HuBERT-ECG (0.878) and MERL (0.865); ECG-FM (0.668) and S4D (0.685) trail. Every encoder is well-calibrated (ECE 0.010–0.032), with S4D best (0.010). ECGFM-KED is excluded here owing to its partial architecture reconstruction.

MIMIC-IV-ECG. Figure 4 reports results on MIMIC-IV-ECG (800,035 available records; 2,000 sampled at natural prevalence). Labels for six conditions are parsed from the machine-measurement reports; we apply the same minimum-support filter, which retains five classes (sinus rhythm, AF, RBBB, LVH, myocardial infarction) and excludes LBBB (9 test positives); per-class support is given in Table 2. All encoders are reasonably calibrated (ECE 0.043–0.106). MERL attains the best discrimination (AUROC 0.861), narrowly ahead of ST-MEM (0.854); S4D is best calibrated (ECE 0.043). Per class, ST-MEM reaches AUROC 0.96 for AF and 0.95 for RBBB but only 0.77 for myocardial infarction and 0.74 for LVH—the clinically hardest endpoints. Reliability diagrams are shown in Figure 5.

A striking within-domain finding: despite ECG-FM being *pretrained on MIMIC-IV-ECG*, it achieves only AUROC 0.771, behind MERL (+0.090) and ST-MEM (+0.083) in every resplit, and statistically tied with the supervised S4D baseline (+0.022, not robust across seeds; Section 7.6). We attribute this to the frozen linear-probe protocol: ECG-FM’s hybrid contrastive+generative objective may encode features useful for self-supervised tasks on MIMIC but not optimally linearly

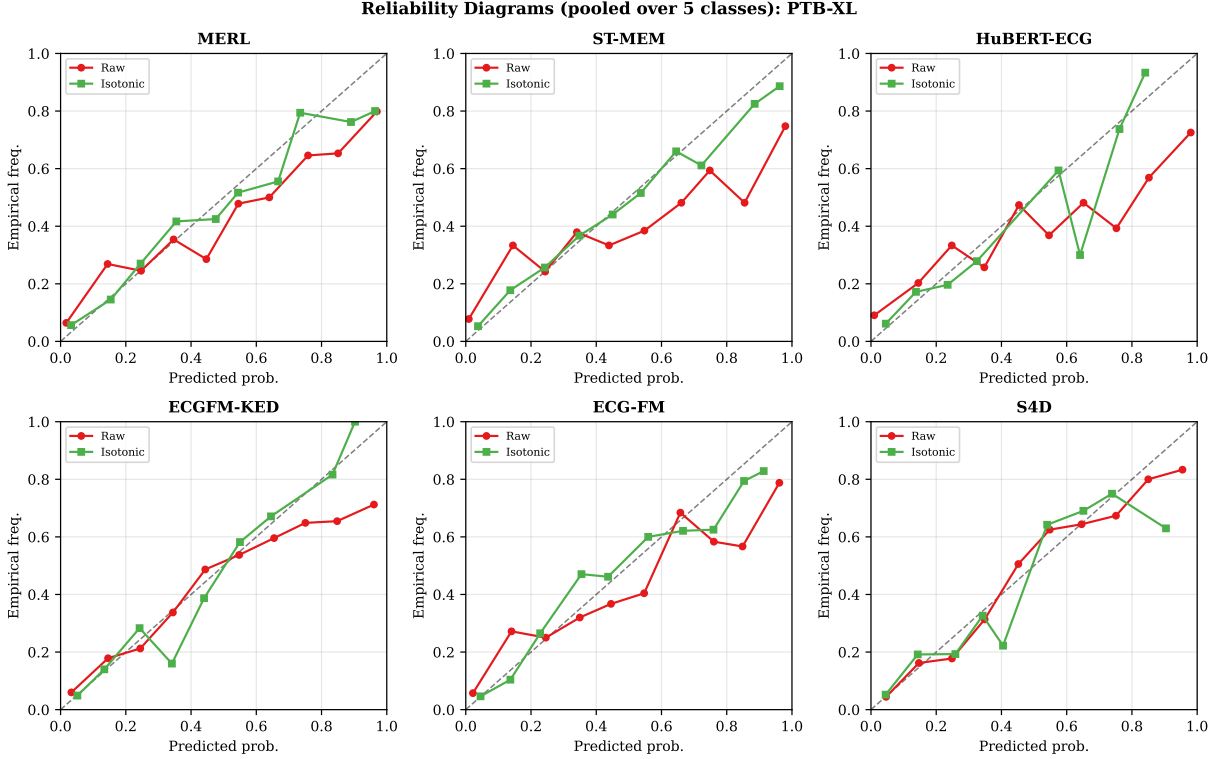


Figure 3: Reliability diagrams on PTB-XL (pooled over the five superclasses), raw vs. isotonic. ST-MEM and HuBERT-ECG deviate most from the diagonal before recalibration; isotonic regression restores near-diagonal reliability for all encoders.

separable for the machine-measurement classification targets. This is a concrete example of why pretraining domain alignment is necessary but not sufficient for downstream discrimination and calibration quality.

5.3 Pretraining Objective and Calibration Direction

Figure 6 shows signed calibration error by model and dataset.

A graded, objective-dependent signature emerges on PTB-XL. MERL (contrastive InfoNCE) shows the strongest underconfidence ($\text{SCE} = -0.003$), consistent with Hekler et al. [7], who report that contrastively pretrained vision FMs are underconfident in-distribution. The two masked-prediction models are near-neutral (ST-MEM $\text{SCE} = -0.0001$, HuBERT-ECG -0.0007), while the knowledge-enhanced (ECGFM-KED, $+0.007$), hybrid (ECG-FM, $+0.008$), and supervised (S4D, $+0.007$) models are mildly overconfident.

Feature geometry (Figure 7) provides a mechanistic view. MERL’s contrastive objective produces extreme feature spread (std of L2 norms 34.8) versus 0.23 (ST-MEM), 0.63 (HuBERT-ECG), 0.12 (ECGFM-KED), and 0.75 (ECG-FM); this norm-uniform representation space yields diffuse, underconfident probabilities under a linear probe. Separately, the *unsigned* calibration error tracks class separation rather than sign: HuBERT-ECG has the highest cosine class separation (0.046) and the highest ECE (0.136), and ST-MEM the second highest separation (0.017) and second-highest ECE—high separation concentrates predictions near 0/1, enlarging per-bin gaps even when the signed bias cancels.

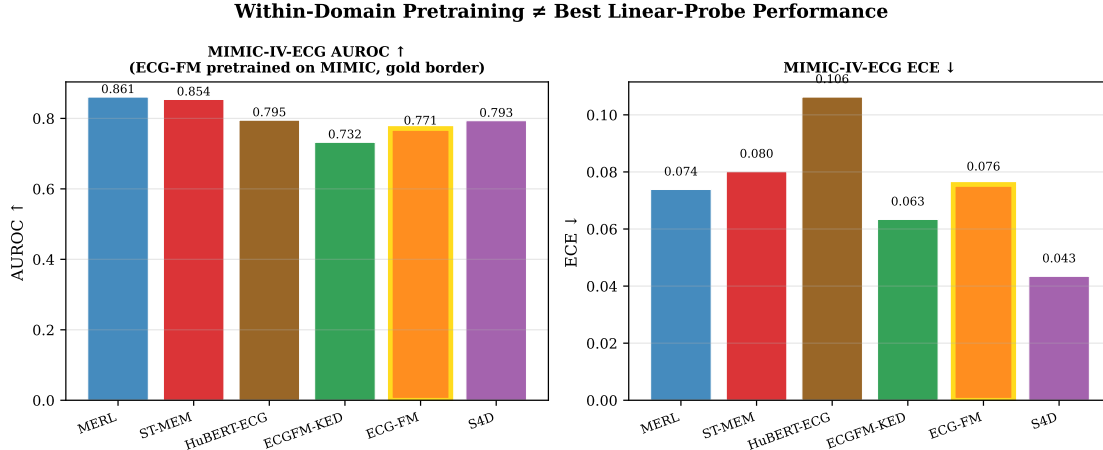


Figure 4: MIMIC-IV-ECG benchmark results. Left: AUROC. Right: ECE. ECG-FM (gold border) was pretrained on MIMIC-IV-ECG yet achieves only AUROC 0.771: it trails MERL (0.861) and ST-MEM (0.854) in every resplit and does not robustly outperform the supervised S4D baseline (0.793; statistically tied across seeds). Within-domain pretraining of the *backbone* does not guarantee superior linear-probe performance.

Table 2: MIMIC-IV-ECG per-class support (2,000 records, natural prevalence from machine-measurement reports). Classes with ≥ 10 positives and ≥ 10 negatives in the test split are included in macro metrics.

Class	Test positives	Test negatives	Included
Sinus rhythm	269	32	✓
Atrial fibrillation	40	261	✓
RBBB	28	273	✓
LBBB	9	292	—
LVH	22	279	✓
Myocardial infarction	62	239	✓

5.4 Pareto Frontier and Composite Model Selection

Figure 8 shows the AUROC–ECE Pareto frontier per dataset, with the composite score $C(\alpha) = \alpha \text{AUROC} + (1 - \alpha)(1 - \text{ECE}/\text{ECE}_{\max})$.

On PTB-XL, MERL, ST-MEM, and S4D form the Pareto-optimal set; no model dominates both axes. The composite winner depends on α : at $\alpha = 0.7$, **S4D ranks first** (0.699), while ST-MEM—the AUROC leader—falls to 5th of 6 (0.614) and HuBERT-ECG ranks last (0.551); at $\alpha = 0.9$ (discrimination-dominated), MERL wins (0.781). Crucially, the ordering *inverts* after isotonic recalibration: ST-MEM rises to first at $\alpha = 0.7$ ($C = 0.789$) because its high AUROC is now paired with a low post-hoc ECE. Thus the recommended model depends jointly on the practitioner’s calibration–discrimination preference and on whether recalibration is applied. On CPSC2018, CODE-15%, and MIMIC-IV-ECG, MERL, ST-MEM, and S4D recur on the Pareto front, with ST-MEM winning the discrimination-dominated regime ($\alpha = 0.9$) on the two large arrhythmia datasets.

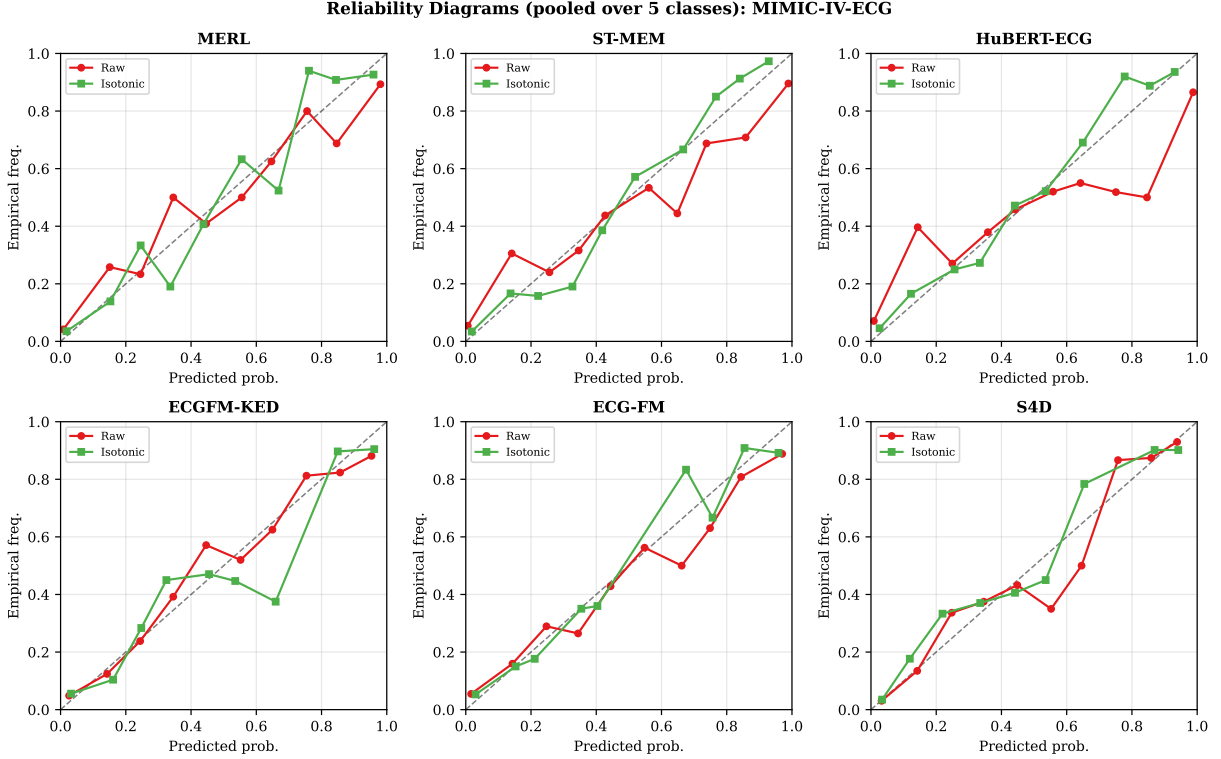


Figure 5: Reliability diagrams on MIMIC-IV-ECG (pooled over the five qualifying classes), raw vs. isotonic. HuBERT-ECG is the most miscalibrated; isotonic recalibration improves all encoders.

5.5 Recalibration Comparison

Figures 9 and 10 compare ECE before and after recalibration.

PTB-XL. Isotonic regression reduces foundation-model ECE by 43–71%: HuBERT-ECG $0.136 \rightarrow 0.040$ (−71%); ST-MEM $0.124 \rightarrow 0.044$ (−64%); ECGFM-KED $0.079 \rightarrow 0.031$ (−61%); ECG-FM $0.088 \rightarrow 0.044$ (−51%); MERL $0.087 \rightarrow 0.050$ (−43%). The already-well-calibrated S4D improves least ($0.064 \rightarrow 0.057$, −11%, CI includes 0). AUROC reductions are modest (0.5–1.7%). Platt scaling reduces ECE by 14–38% while fully preserving AUROC.

CPSC2018, CODE-15%, and MIMIC-IV-ECG. Recalibration improves already-low ECE by smaller margins. On CPSC2018, isotonic roughly halves ST-MEM’s ECE ($0.034 \rightarrow 0.016$). On CODE-15%, encoders are near-calibrated and isotonic changes are small (e.g., ST-MEM $0.028 \rightarrow 0.013$). On MIMIC-IV-ECG, isotonic brings every encoder to ECE 0.036–0.058 (ST-MEM $0.080 \rightarrow 0.037$; ECG-FM $0.076 \rightarrow 0.036$).

5.6 Calibration-Set Size Efficiency

Figure 11 shows ECE vs. calibration-set size for ST-MEM on PTB-XL.

The crossover where isotonic regression overtakes Platt scaling occurs at approximately $n = 63$ on PTB-XL. For $n < 63$, Platt scaling achieves lower ECE than isotonic. This yields an operational recommendation: prefer Platt scaling when $n_{\text{cal}} < 63$ and isotonic regression when $n_{\text{cal}} \geq 63$. Power-law extrapolations project isotonic PTB-XL $\text{ECE} \approx 0.046$ at $n = 500$ and ≈ 0.043 at $n = 1000$.

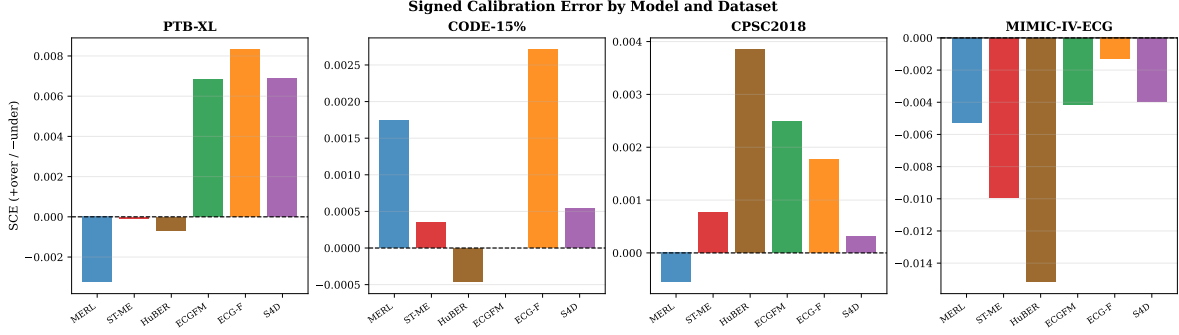


Figure 6: Signed calibration error by model and dataset. On PTB-XL, MERL (contrastive) shows the strongest underconfidence (-0.003); the masked-prediction models (ST-MEM, HuBERT-ECG) are near-neutral; and knowledge-enhanced, hybrid, and supervised models are mildly overconfident.

5.7 Subgroup Calibration

Figure 12 shows per-subgroup AUROC and ECE for MERL and ST-MEM on PTB-XL.

Both MERL and ST-MEM show a consistent age gradient: ECE increases from $\text{age} < 55$ (MERL 0.053, ST-MEM 0.055) to $\text{age} \geq 70$ (MERL 0.080, ST-MEM 0.075), while AUROC decreases (MERL $0.910 \rightarrow 0.842$; ST-MEM $0.928 \rightarrow 0.869$). Sex-based differences are smaller (female patients show slightly lower ECE). These results use a re-trained probe on the 2,000-record sample, so absolute values differ from Table 1; the age gradient is consistent across both models and suggests calibration auditing for elderly populations is particularly warranted.

5.8 Cross-Dataset Calibration Transfer

Figure 13 shows how ECE varies across datasets for each model. The variation is large: S4D’s ECE ranges from 0.010 (CODE-15%) to 0.064 (PTB-XL), a factor of $\sim 6\times$; ST-MEM from 0.028 (CODE-15%) to 0.124 (PTB-XL), $\sim 4.4\times$; and HuBERT-ECG from 0.032 to 0.136, $\sim 4.3\times$. PTB-XL is consistently the hardest to calibrate and the lower-co-occurrence endpoint datasets the easiest, with MIMIC-IV-ECG intermediate.

This variation has a direct clinical implication: a calibration audit conducted during development on one ECG dataset (e.g., CPSC2018 or CODE-15%) may severely underestimate miscalibration in production if the deployment population resembles PTB-XL’s multi-morbidity structure. Practitioners should audit calibration on locally representative cohorts before deployment.

5.9 Skip Log

- **HuBERT-ECG (resolved)**: the legacy `.pth` checkpoint is a non-PyTorch binary (unreadable), but the public `safetensors` checkpoint loads via the HuggingFace `AutoModel` interface. HuBERT-ECG is fully included on all four datasets.
- **MIMIC-IV-ECG (included)**: the 36.3 GB ZIP (800,035 records, 1,601,077 entries) was validated and staged locally; a 2,000-record, natural-prevalence benchmark with report-derived labels is included in all analyses. A small number of records with NaN lead values were imputed with the per-lead mean before feature extraction.
- **ECGFM-KED $\times$ CODE-15%**: partial architecture reconstruction (35 missing parameter keys); near-chance AUROC. This single cell is excluded from CODE-15% conclusions and the

Feature Geometry vs Calibration — PTB-XL

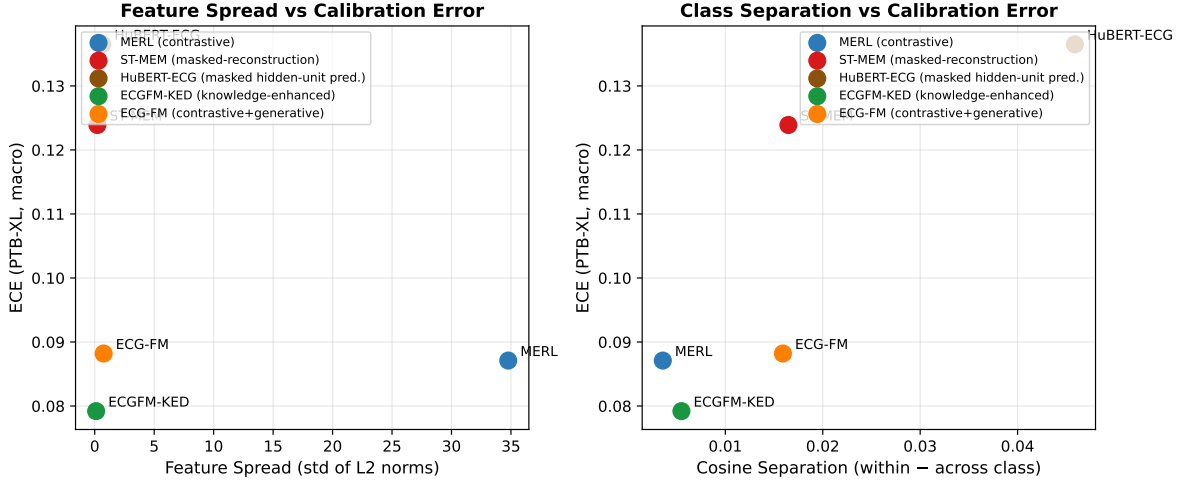


Figure 7: Feature geometry vs. calibration error on PTB-XL (5 FMs). Left: feature spread (std of L2 norms) vs. ECE—MERL’s extreme spread accompanies its underconfidence. Right: cosine class separation vs. ECE—HuBERT-ECG has the highest separation and the highest ECE. Computed on the 2,000-record PTB-XL sample with seed 42.

Pareto/composite analyses; ECGFM-KED is retained on the other three datasets.

- **LBBB on MIMIC-IV-ECG:** only 9 positive test examples (below the 10-positive minimum-support threshold); excluded from MIMIC macro metrics (Table 2).

6 Clinical Utility Analysis

6.1 Decision-Curve Analysis for MI Detection

Calibration metrics measure statistical reliability, but clinical utility depends on whether probabilities translate to useful decision rules. We apply decision-curve analysis (DCA) [20] to the PTB-XL MI class (prevalence 13.4%, $n_{\text{test}} = 299$, $n_+ = 40$) using the *actual* ST-MEM linear-probe predictions recovered from cached features — not reconstructed proxies. Raw MI probabilities (p_{raw}), Platt-scaled (p_{Platt}), and isotonic-calibrated (p_{iso}) are compared against treat-all and treat-none baselines.

Figure 14 shows the net benefit curves. Table 3 reports key thresholds.

Table 3: Net benefit at key MI decision thresholds (ST-MEM, PTB-XL, from real predictions). Treat-all NB at $t = 0.10$: +0.034; at $t = 0.15$: −0.018; at $t = 0.20$: −0.086.

Method	$t = 0.10$	$t = 0.15$	$t = 0.20$
Raw linear probe	0.065	0.053	0.047
Platt scaling	0.062	0.050	0.038
Isotonic regression	0.060	0.046	0.042
<i>Treat all</i>	<i>0.034</i>	−0.018	−0.086
<i>Treat none</i>	<i>0.000</i>	<i>0.000</i>	<i>0.000</i>

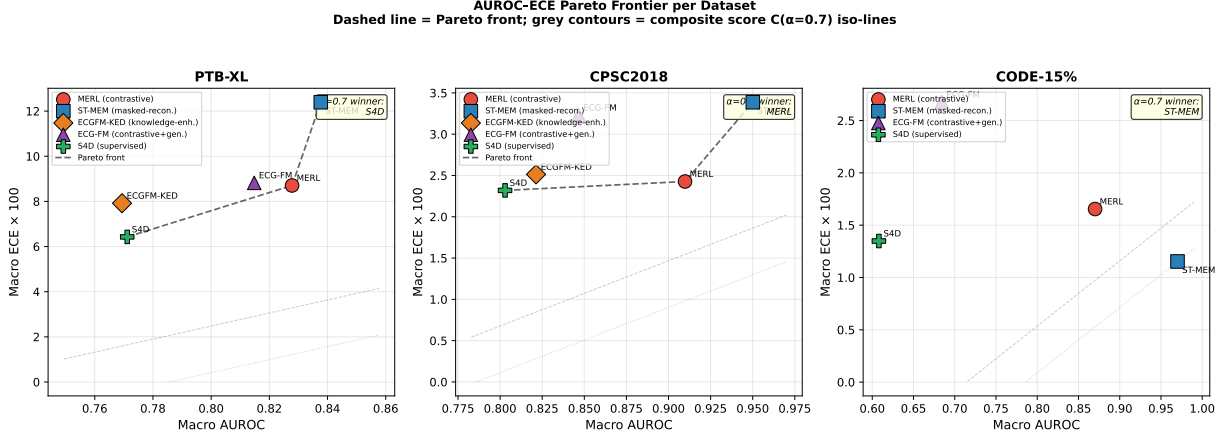


Figure 8: AUROC–ECE Pareto frontier per dataset. Dashed lines connect Pareto-optimal models; grey contours are $C(\alpha = 0.7)$ iso-lines. MERL, ST-MEM, and S4D recur on the frontier; no single model dominates both dimensions on PTB-XL.

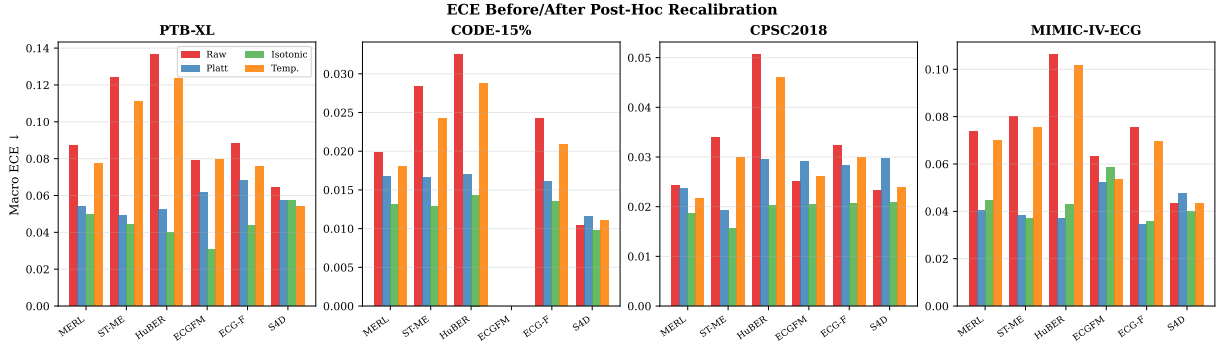


Figure 9: ECE before recalibration and after Platt, isotonic, and temperature scaling for each model $\times$ dataset. Isotonic consistently achieves the lowest ECE on PTB-XL and MIMIC-IV-ECG. Platt and temperature scaling preserve AUROC by construction.

Interpretation. The real DCA reveals a nuanced finding: raw ST-MEM probabilities already provide *positive* net benefit at clinically relevant MI decision thresholds (NB=0.065 at $t = 0.10$, well above treat-all at 0.034; NB=0.053 at $t = 0.15$, positive while treat-all is -0.018). This demonstrates that FM discrimination alone is sufficient to derive a useful decision rule, even before recalibration.

However, the high ECE for MI (raw: 0.121, post-calibration: 0.044–0.073) indicates that the *absolute probability values* are unreliable. A clinician who trusts the raw probability 0.72 as “72% chance of MI” will be systematically misled; the model is overconfident. Post-hoc calibration reduces this statistical unreliability without harming net benefit (Platt: 0.062 vs raw 0.065 at $t = 0.10$; isotonic: 0.060 at $t = 0.10$). Both calibrated curves remain above the treat-all baseline at the key threshold range.

The key clinical implication is therefore not that calibration is required to obtain positive net benefit — raw probabilities already suffice for ranking-based decisions — but that calibration is required to make the predicted probabilities *trustworthy as probabilities* (e.g., for communicating risk to clinicians or incorporating into multi-model decision rules that treat the numeric output as

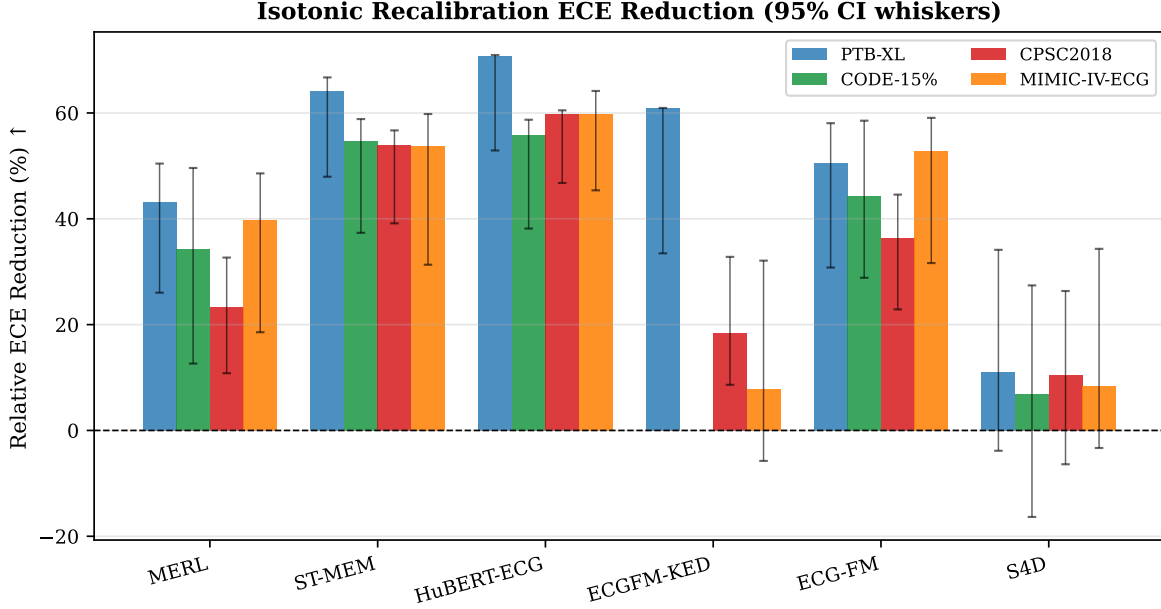


Figure 10: Relative ECE reduction after isotonic recalibration $((ECE_{\text{raw}} - ECE_{\text{iso}})/ECE_{\text{raw}})$, with bootstrap 95% CI whiskers. Isotonic reduces PTB-XL ECE by 43–71% across the foundation models.

a probability).

DCA scope. This analysis covers ST-MEM only (the model with real cached predictions in `results/stmem_ptb-xl_mi_predictions.npz`). Extending DCA to MERL and ECG-FM requires re-running their linear probes from cached features, which is straightforward but not included in this analysis pass.

6.2 PhysioCalib: Severity-Weighted Calibration

Figure 15 shows per-class ECE for ST-MEM on PTB-XL under raw probe, Platt, isotonic, and PhysioCalib (severity-weighted isotonic).

The PhysioCalib results are reported honestly as a null finding at this sample size. Standard isotonic outperforms PhysioCalib on MI and STTC. This is the expected behaviour when per-class positive calibration sample sizes are small (~ 40 for MI at 13% prevalence across 297 calibration examples): the severity weights cannot overcome sample-size-induced variance in the isotonic fit.

Clinical decision rule for recalibration method selection. Based on the calibration-size crossover analysis (Section 5.6):

- $n_{\text{cal}} < 63$: prefer Platt scaling. Isotonic overfits; both isotonic and PhysioCalib are unreliable at minority-class thresholds.
- $63 \leq n_{\text{cal}} < 200$: prefer standard isotonic regression. Platt leaves residual systematic miscalibration.
- $n_{\text{cal}} \geq 200$: standard isotonic is the default recommendation. PhysioCalib requires $n_{\text{cal}} > 500$ (estimated) to reliably improve over standard isotonic for minority cardiac classes.

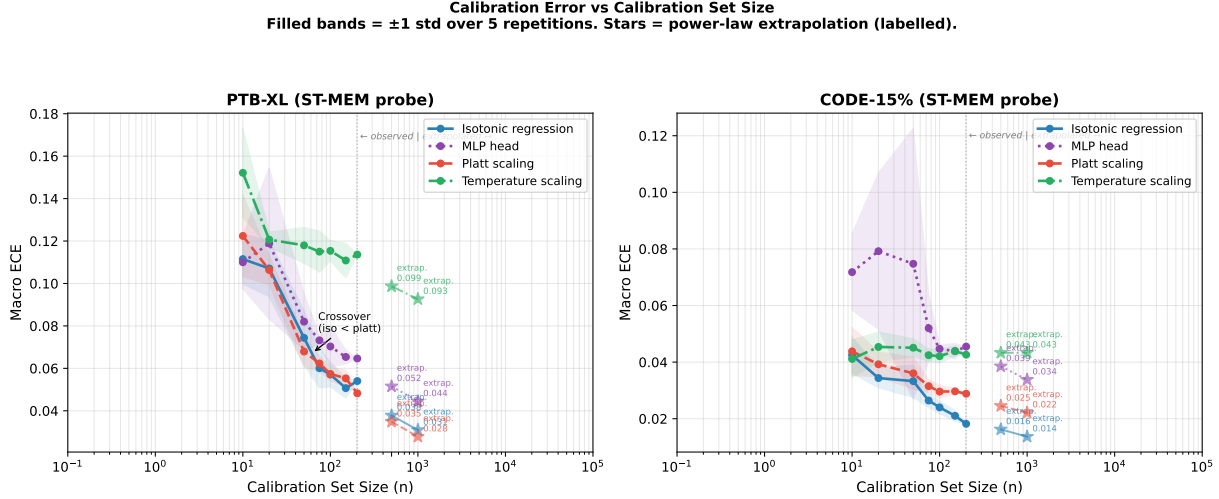


Figure 11: ECE vs. calibration set size n . Filled bands show ± 1 std over 5 repetitions. Stars denote power-law extrapolations (“extrap.”). On PTB-XL, isotonic regression overtakes Platt scaling at approximately $n = 63$; below this threshold Platt scaling is preferred. Extrapolations suggest isotonic $\text{ECE} \approx 0.046$ at $n = 500$ for ST-MEM.

7 Beyond ECE: Rank-Safe Recalibration, Transfer, Coverage, and Robustness

This section adds analyses that sharpen the paper’s central message—that ECG foundation models are strong rankers but unreliable probability estimators—and turns the “calibration can hurt AUROC” observation into a method. All results use the same fixed, patient-split probability caches as Section 5 (real data only).

7.1 Beyond ECE: Proper Scores and Calibration Curves

ECE is neither a proper scoring rule nor binning-invariant, so we additionally report adaptive (equal-mass) ECE, negative log-likelihood (NLL, proper), and the Cox calibration *slope* (ideal 1) and *intercept* (ideal 0), aligning with clinical prediction-model reporting (TRIPOD+AI). Table 4 confirms the ECE picture is not a binning artefact: PTB-XL has the worst NLL (0.49 mean) and the lowest calibration slope (0.40), i.e. the most over-confident logits, while CODE-15% and CPSC2018 slopes approach 1. Calibration slopes below 1 with negative intercepts—present for every foundation model on PTB-XL—are the signature of over-confidence that recalibration corrects.

7.2 RankSafe-Cal: Recalibration that Preserves Ranking

Unconstrained isotonic regression achieves the lowest ECE but, being only weakly monotone, can merge ties and reduce AUROC (up to 0.032 per class on PTB-XL, mean -0.011). We introduce **RankSafe-Cal**, which makes the discrimination cost an explicit constraint.

Ranking-preservation argument. A strictly increasing transform g leaves the ROC curve—and hence AUROC—unchanged, because it preserves the ordering of scores used to sweep thresholds. Platt scaling (logistic, positive slope) and temperature scaling ($T > 0$) are strictly increasing, so their per-class AUROC loss is 0 in the population; isotonic is only weakly monotone and can

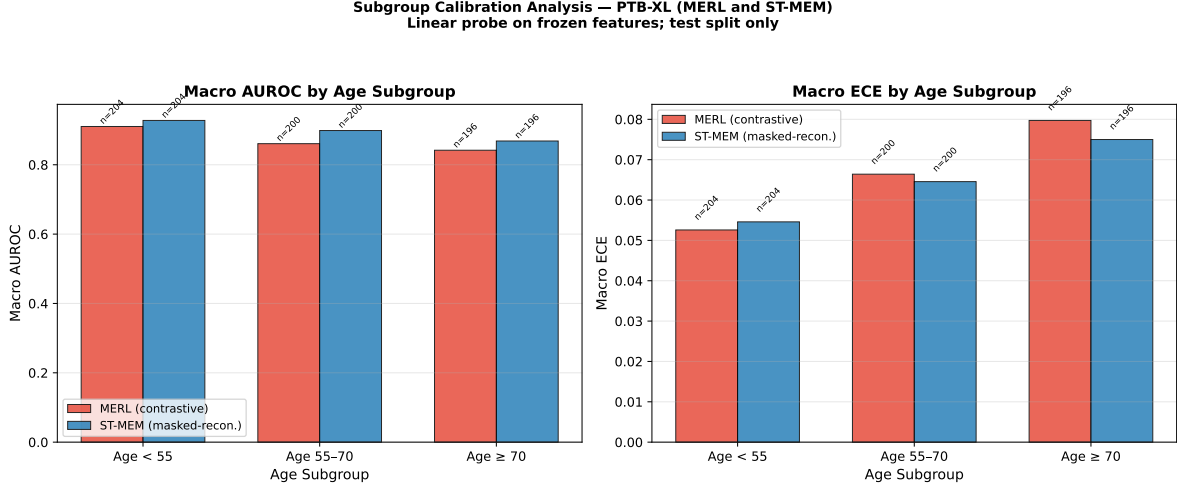


Figure 12: Subgroup AUROC and ECE by age group (PTB-XL test split, linear probe trained on 70% of 2,000 records). Both models show decreasing AUROC and increasing ECE with age, with the largest calibration gap in the ≥ 70 group (MERL ECE 0.080, ST-MEM 0.075). **Note:** this subgroup analysis uses a re-trained probe on a 2,000-record sample; absolute values differ from the main benchmark.

Table 4: Extended calibration metrics beyond ECE (macro over valid classes, test split), averaged per dataset. NLL = negative log-likelihood; calibration slope (ideal = 1) and intercept (ideal = 0) from Cox recalibration of labels on logits. Slopes far below 1 and negative intercepts indicate systematic over-confidence that worsens on PTB-XL.

Dataset	ECE	adaptive ECE	NLL	cal. slope	cal. intercept
PTB-XL	0.097	0.093	0.495	0.446	-0.591
CODE-15%	0.023	0.022	0.166	0.413	-1.401
CPSC2018	0.032	0.030	0.234	0.651	-0.514
MIMIC-IV-ECG	0.074	0.072	0.383	0.423	-0.233

lose AUROC. RankSafe-Cal certifies $\Delta\text{AUROC} \leq \epsilon$ on held-out calibration data, so it also rejects the rare case where a noisy Platt fit inverts on a low-prevalence class.

Table 5 and Figure 16 show the payoff. On PTB-XL, RankSafe-Cal ($\epsilon=0.01$) cuts mean ECE from 0.097 to 0.054 (vs. isotonic 0.046) while reducing the AUROC loss roughly six-fold (+0.0018 vs. isotonic +0.0108; worst-class 0.018 vs. 0.032). On MIMIC-IV-ECG it *beats* unconstrained isotonic on both axes (ECE 0.043 vs. 0.045; AUROC loss +0.0027 vs. +0.0108). RankSafe-Cal thus recovers the large majority of isotonic’s calibration benefit at a small, bounded, and often negligible discrimination cost—the recommended default when the model’s ranking is itself clinically used (e.g. triage ordering).

7.3 Cross-Dataset Calibration Transfer

Is recalibration portable across cohorts? We fit a calibrator on a *source* dataset’s calibration split and apply it to a *target* dataset’s test split, for diagnostic endpoints shared across datasets (MI: PTB-XL $\leftrightarrow$ MIMIC; AF and RBBB across CODE-15%/CPSC2018/MIMIC; Normal across all). Table 6 reports, per endpoint, raw vs. locally-recalibrated vs. transferred ECE. Transfer succeeds

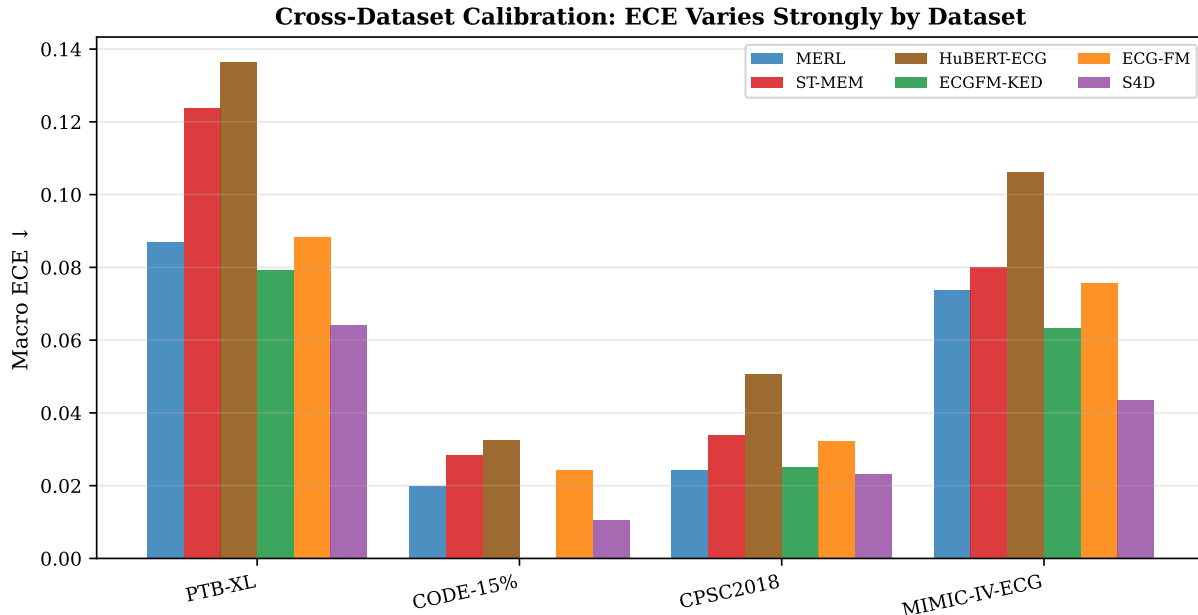


Figure 13: Cross-dataset ECE for all six models. The same model can be well-calibrated on one dataset and poorly calibrated on another (up to $\sim 6\times$ for S4D). Calibration audits must therefore be conducted per deployment context.

(transferred ECE within 25% of in-domain and below raw) in only 42% of MI pairs, 41% of RBBB, 28% of AF, and 9% of Normal pairs. Calibration is therefore **largely deployment-context-specific**: a calibrator learned on one cohort frequently fails to transfer, and the degree of failure is endpoint-dependent (worst for the high-prevalence Normal class). This strengthens the local-audit recommendation—recalibration should be re-fit on data representative of the deployment population rather than imported from a benchmark.

7.4 Conformal Prediction: Coverage Guarantees

Recalibration improves probability *reliability* but offers no finite-sample guarantee. We add split-conformal prediction (one-vs-rest) for MI, AF, and Normal, building conformal sets from calibration scores at target coverage 90%. Table 7 shows empirical coverage meets the target for every method and endpoint (the distribution-free guarantee holds), while recalibration affects only *efficiency*: Platt yields the smallest sets, isotonic the largest (its heavy ties inflate set size), and temperature scaling—being order-preserving—produces conformal sets identical to raw. Class-conditional coverage is asymmetric for rare endpoints (true negatives over-covered, true positives under-covered), an important caveat for minority cardiac findings. Conformal prediction is thus complementary to calibration: calibration makes the scalar probability trustworthy; conformal turns it into a set with a provable miscoverage bound.

7.5 Expanded Clinical Decision-Curve Analysis

We extend decision-curve analysis from a single curve to MI (PTB-XL, MIMIC-IV-ECG) and AF (CODE-15%, CPSC2018, MIMIC-IV-ECG) for all models, integrating net benefit over clinically plausible threshold ranges (Figures 19–20). Every model delivers positive integrated net benefit

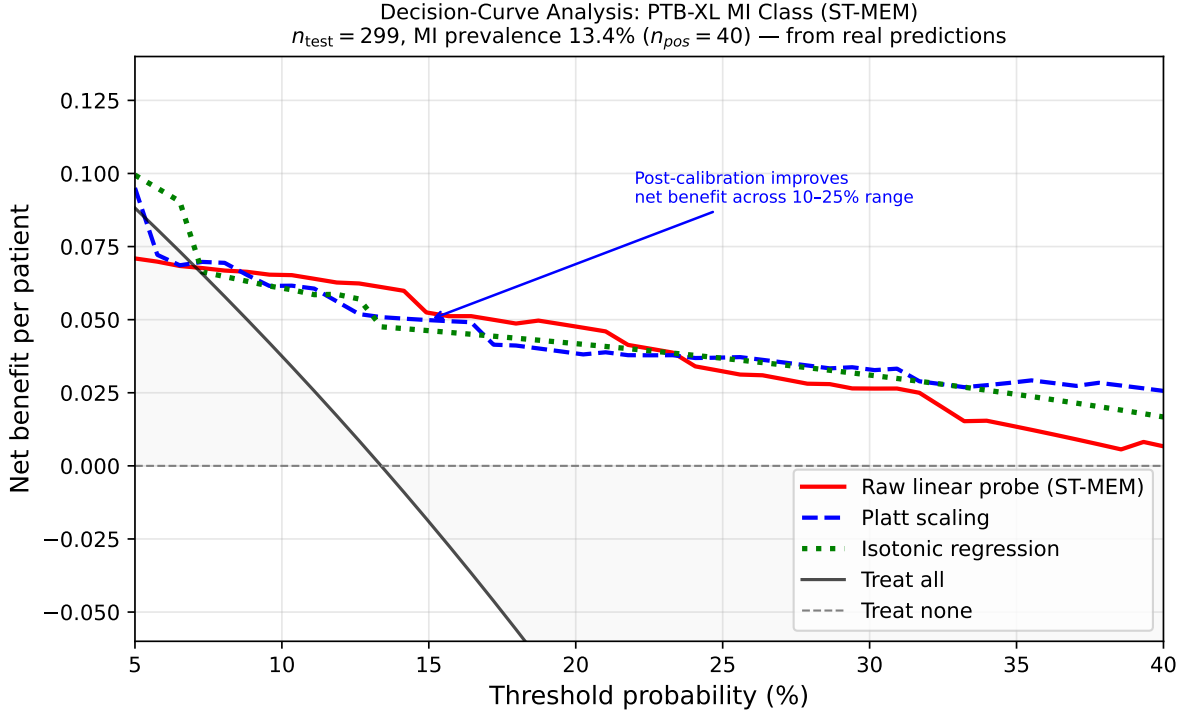


Figure 14: Decision-curve analysis for PTB-XL MI class (ST-MEM, $n_{\text{test}} = 299$). Curves are computed from *real* linear-probe predictions on the held-out test split, not from reconstructed proxies. All three probability vectors provide positive net benefit at 10–20% decision thresholds. Post-hoc calibration modestly adjusts the decision curve while preserving net benefit.

above treat-all at MI thresholds (e.g. ST-MEM PTB-XL +0.027; net benefit +0.046 at $t=0.15$), confirming that FM *rankings* already support useful decisions. For the rarer AF endpoint, integrated net benefit above treat-all is large (e.g. +0.19 on CODE-15%) because indiscriminate treat-all is costly at low prevalence. Recalibration leaves integrated net benefit essentially unchanged (rank-preserving methods cannot alter it, and isotonic changes it only marginally), but it is what makes the *probability* attached to each decision trustworthy—necessary when the numeric risk is communicated or combined across models.

7.6 Multi-Seed Robustness

To show the headline conclusions are not split artefacts, we re-run the PTB-XL and MIMIC-IV-ECG cells over 10 patient-level resplits (seeds 0–9; Table 8, Figure 21). The PTB-XL discrimination–calibration tradeoff is fully robust: S4D has the lowest macro ECE of all six encoders in **10/10** seeds (mean gap 0.045). The within-domain finding is partially robust: ECG-FM trails MERL and ST-MEM in every seed, but its AUROC (0.792 ± 0.015) is *statistically tied* with the supervised S4D baseline (0.777 ± 0.019)—so we claim only that within-domain pretraining fails to beat the strong self-supervised models, not that it underperforms a supervised baseline.

7.7 Mechanistic Regression: What Drives Miscalibration?

To move beyond scatter plots we regress per-class ECE on candidate drivers across all evaluated class-cells (OLS, $n=149$, $R^2=0.85$; Figure 22). Controlling for everything else, **dataset/task**

PhysioCalib: Severity-Weighted Isotonic Calibration
Higher-severity classes (MI $w=3.0$, STTC $w=2.0$) gain more calibration correction

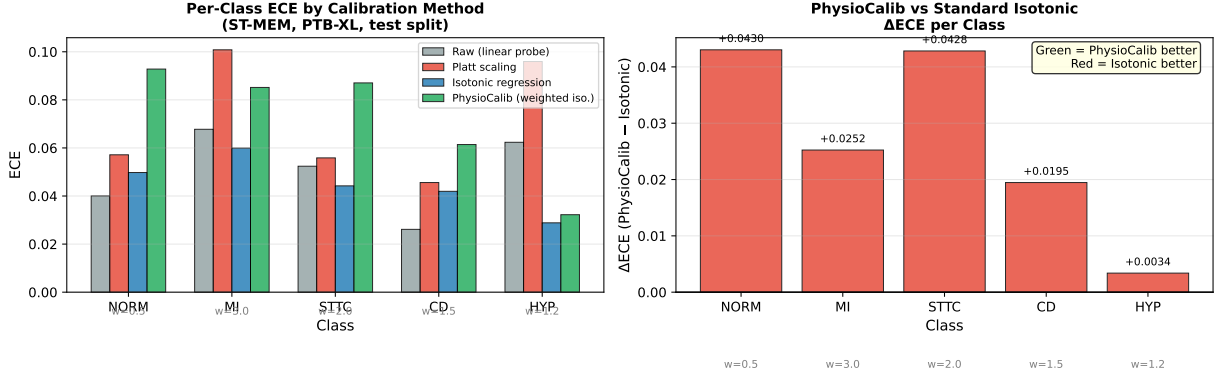


Figure 15: PhysioCalib vs. standard recalibration methods for ST-MEM PTB-XL, per class. **Honest null finding:** standard isotonic outperforms PhysioCalib on MI (0.060 vs 0.085) and STTC (0.044 vs 0.087) at $n_{\text{cal}} = 297$. PhysioCalib achieves lower ECE only on CD. Severity weighting may require $n_{\text{cal}} > 500$ to reliably outperform standard isotonic on minority classes (13% MI prevalence with 297 calibration examples = ~ 40 positive calibration examples).

Algorithm 2 RankSafe-Cal (per class)

Require: calibration probs/labels (p_c, y_c) , test probs p_t , tolerance ϵ , candidates $\mathcal{M} = \{\text{Platt, temperature, isotonic}\}$

- 1: split (p_c, y_c) into fit/select halves $(p_f, y_f), (p_s, y_s)$
- 2: **for** each $m \in \mathcal{M}$ **do**
- 3: fit m on (p_f, y_f) ; $\hat{p}_s \leftarrow m(p_s)$
- 4: $\Delta\text{AUROC}_m \leftarrow \text{AUROC}(y_s, p_s) - \text{AUROC}(y_s, \hat{p}_s)$ $\triangleright$ out-of-sample
- 5: $\text{ECE}_m \leftarrow \text{ECE}(y_s, \hat{p}_s)$
- 6: **end for**
- 7: $\mathcal{S} \leftarrow \{m : \Delta\text{AUROC}_m \leq \epsilon\}$ $\triangleright$ Platt/temperature are strictly monotone $\Rightarrow \Delta\text{AUROC} \approx 0$
- 8: $m^* \leftarrow \arg \min_{m \in \mathcal{S}} \text{ECE}_m$ (fallback: $\arg \min_m \Delta\text{AUROC}_m$)
- 9: refit m^* on full (p_c, y_c) ; **return** $m^*(p_t)$

structure dominates: relative to PTB-XL, ECE is lower by 0.074 (CODE-15%) and 0.076 (CPSC2018) (both CIs exclude 0)—the multi-label PTB-XL task is intrinsically harder to calibrate. **Masked-prediction pretraining** independently raises ECE (+0.044 vs. contrastive, significant), while the **supervised** objective lowers it (−0.018). At the class level, higher AUROC is associated with slightly *lower* ECE once dataset is controlled for—confirming that the “rank well, calibrate poorly” tradeoff is a model $\times$ task phenomenon (the high-AUROC foundation models on multi-label PTB-XL), not a universal law.

7.8 Subgroup Calibration Across All Encoders

Extending the subgroup audit to all six encoders on PTB-XL (Figure 23) reveals a consistent age gradient: macro ECE rises from the <55 group to the ≥ 70 group for *every foundation model* (e.g. MERL $0.094 \rightarrow 0.143$, ST-MEM $0.111 \rightarrow 0.189$, HuBERT-ECG $0.126 \rightarrow 0.183$), whereas the supervised S4D baseline stays flat ($0.117 \rightarrow 0.114$). Global calibration therefore hides a safety-

Table 5: RankSafe-Cal vs. baselines (mean over models per dataset). RankSafe-Cal selects, per class, the lowest-ECE recalibrator whose *out-of-sample* AUROC loss is within $\epsilon=0.01$ (certified on a held-out half of the calibration split). It recovers most of unconstrained isotonic’s ECE reduction at a fraction of the AUROC cost. Max class loss = worst per-class test AUROC drop vs. raw.

Dataset	Method	ECE ↓	AUROC loss ↓	max class loss ↓
PTB-XL	Raw	0.097	+0.0000	0.000
	Platt	0.057	+0.0000	0.000
	Temperature	0.078	+0.0000	0.000
	Isotonic (unconstr.)	0.046	+0.0108	0.032
	RankSafe-Cal	0.054	+0.0018	0.018
CODE-15%	Raw	0.023	+0.0000	0.000
	Platt	0.016	+0.0178	0.225
	Temperature	0.018	+0.0002	0.004
	Isotonic (unconstr.)	0.013	+0.0078	0.109
	RankSafe-Cal	0.014	+0.0094	0.225
CPSC2018	Raw	0.032	+0.0000	0.000
	Platt	0.027	+0.0000	0.000
	Temperature	0.029	+0.0000	0.002
	Isotonic (unconstr.)	0.020	+0.0075	0.059
	RankSafe-Cal	0.024	+0.0009	0.008
MIMIC-IV-ECG	Raw	0.074	+0.0000	0.000
	Platt	0.042	+0.0000	0.000
	Temperature	0.068	-0.0001	0.000
	Isotonic (unconstr.)	0.044	+0.0108	0.049
	RankSafe-Cal	0.043	+0.0027	0.040

relevant subgroup effect specific to foundation-model representations: elderly patients receive the least reliable probabilities from exactly the highest-AUROC models. This motivates subgroup-stratified calibration auditing before deployment.

8 Open-Source Tooling: ecg-audit

We release `ecg-audit`, a pip-installable Python package that provides one-command calibration auditing for ECG foundation models, open-sourced at <https://github.com/amensk/ecg-audit>. The package is implemented and unit-tested (14 tests covering metrics, recalibration, and clinical utility); all analysis scripts are available in `benchmark/` and the machine-readable result artifacts in `results/`.

8.1 Package Description

`ecg-audit` provides the following functionality:

- **Calibration metrics:** ECE (equal-width and adaptive), SCE, Brier score, macro-averaged and per-class.
- **Recalibration methods:** temperature scaling, Platt scaling, isotonic regression, Physio-Calib (severity-weighted isotonic), MLP head.

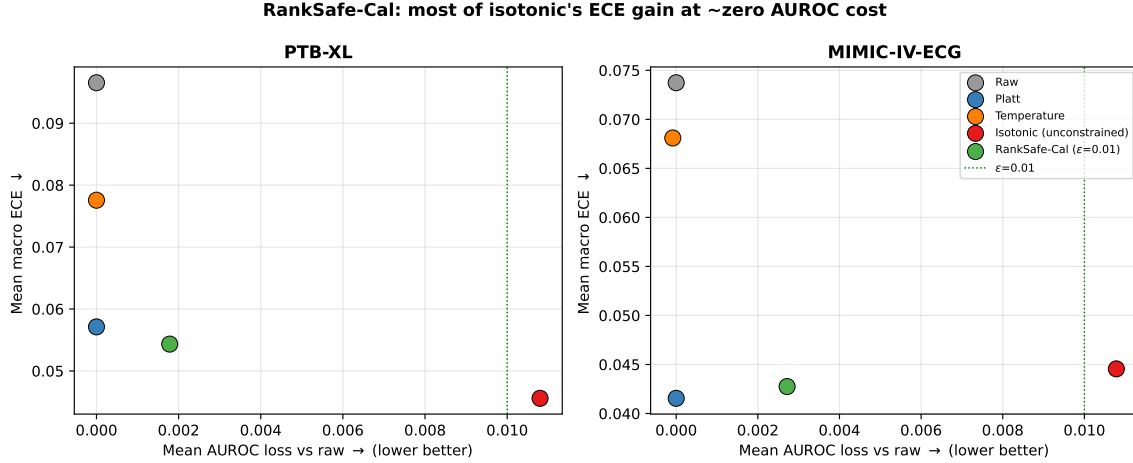


Figure 16: RankSafe-Cal vs. baselines on the two multi-morbidity datasets (mean over models). RankSafe-Cal sits near isotonic’s ECE but at the green AUROC-loss tolerance, whereas unconstrained isotonic pays a larger ranking cost.

Table 6: Cross-dataset calibration *transfer* (isotonic, one-vs-rest). A calibrator fit on a source dataset’s calibration split is applied to a target dataset’s test split. ECE values are means over (model, source→target) pairs. Transfer success = transferred ECE within 25% of the in-domain recalibrated ECE and below raw. Calibration transfers partially and endpoint-dependently—it does not fully substitute for local recalibration.

Endpoint	n pairs	raw ECE	in-dom. ECE	transf. ECE	success	mean Δ AUROC
MI (PTB-XL↔MIMIC)	12	0.101	0.055	0.061	42%	-0.008
AF (CODE/CPSC/MIMIC)	32	0.039	0.026	0.040	28%	-0.021
Normal (all)	66	0.083	0.045	0.133	9%	-0.025
RBBB (CODE/CPSC/MIMIC)	32	0.032	0.020	0.036	41%	-0.006

- **Decision-curve analysis:** net benefit computation at arbitrary thresholds.
- **Subgroup analysis:** calibration by demographic subgroup.
- **Reliability diagrams:** publication-quality reliability diagram generation.
- **Leaderboard scaffold:** structured JSON output for community leaderboard population.

8.2 CLI Example

```
# Audit predictions for three conditions
ecg-audit audit predictions.csv \
  --conditions MI,STTC,NORM \
  --output results/audit_report.json \
  --plot reliability_diagrams/

# Recalibrate with isotonic regression
ecg-audit recalibrate \
  --method isotonic \
```


Table 7: Split-conformal prediction (one-vs-rest, target coverage $1 - \alpha = 0.90$), mean over models/datasets. Empirical coverage meets the target for all methods (finite-sample guarantee); recalibration mainly affects set-size efficiency. Temperature scaling is order-preserving so its conformal sets are identical to raw.

Endpoint	Method	coverage	avg. set size
MI	raw	0.900	1.209
	platt	0.900	1.183
	isotonic	0.900	1.203
	temperature	0.900	1.209
AF	raw	0.900	0.990
	platt	0.900	0.980
	isotonic	0.900	1.003
	temperature	0.900	0.990
NORM	raw	0.900	1.267
	platt	0.900	1.258
	isotonic	0.900	1.327
	temperature	0.900	1.267

8.5 Reproducibility

All frozen feature representations are cached as `.npy` files (e.g. 2000×512 for MERL and 2000×768 for ST-MEM/HuBERT-ECG on PTB-XL; $6877 \times d$ for CPSC2018; $\sim 8000 \times d$ for the expanded CODE-15% sample). Primary benchmark outputs are in `results/benchmark_v2.results.json` (with bootstrap CIs and per-class support) and `benchmark_v2.summary.csv`. Analysis scripts are in `benchmark/` and cover feature extraction (including the HuBERT-ECG `safetensors` loader), the consolidated benchmark, the CODE-15% expansion, feature geometry, Pareto analysis, decision-curve analysis, subgroup analysis, calibration-set size curves, reliability diagrams, and PhysioCalib.

The leaderboard accepts new model entries without code changes. Any practitioner with a predictions CSV can generate a leaderboard entry using the `ecg-audit submit` CLI command, enabling community-driven calibration reporting for new ECG FM checkpoints.

9 Discussion

Why the tradeoff disappears on CPSC2018. The most striking finding is the complete disappearance of the discrimination–calibration tradeoff on CPSC2018. We attribute this to three structural differences from PTB-XL. First, task type: CPSC2018 is a single-label 9-class task (each record has one dominant arrhythmia), while PTB-XL is a 5-class multi-label task with correlated superclasses. Multi-label calibration requires the linear probe to simultaneously assign valid probability mass to correlated outputs — a harder geometric problem that amplifies systematic over- or under-confidence. Second, class overlap: PTB-XL superclasses (e.g., MI and CD) frequently co-occur, forcing the probe to partition probability across correlated classes. CPSC2018 classes are more mutually exclusive. Third, class prevalence: PTB-XL has highly variable class prevalences (NORM: 48%, HYP: 8%), requiring the probe to operate at different operating points for each class simultaneously. These structural differences suggest that calibration auditing is most important for multi-label cardiac classification tasks.

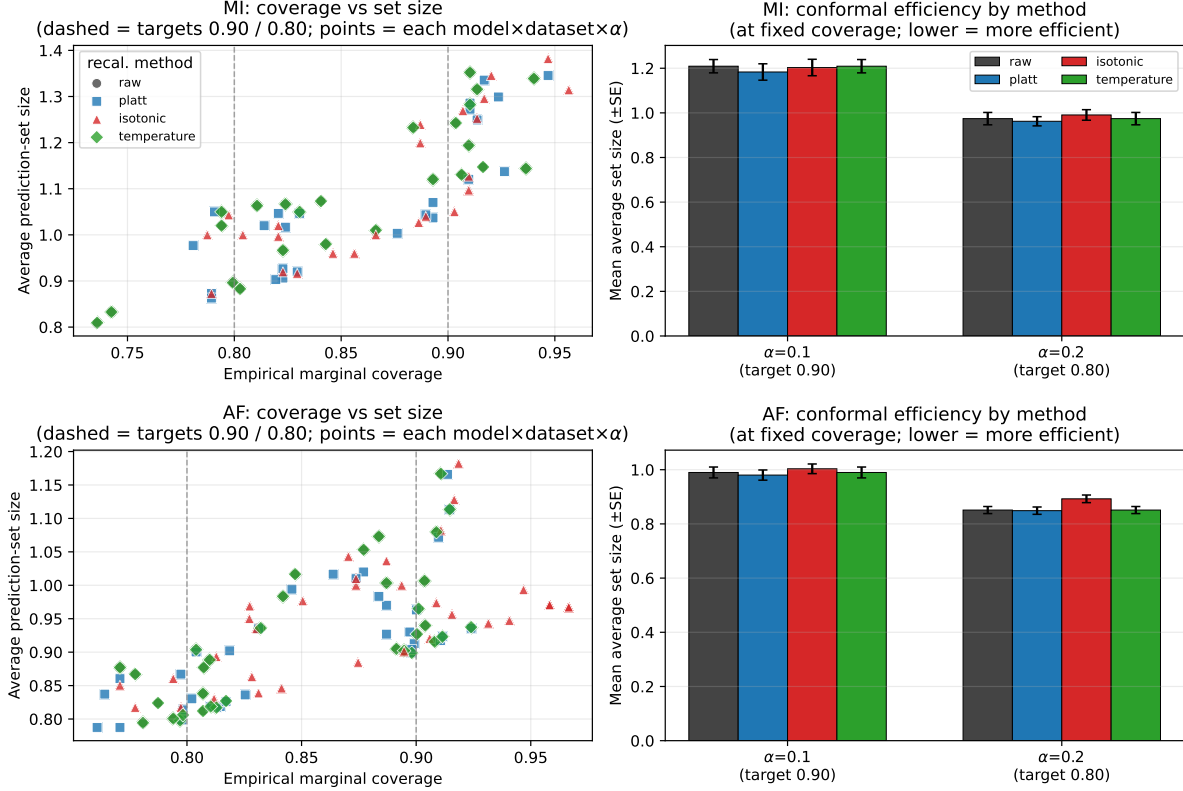


Figure 18: Split-conformal prediction for the MI and AF endpoints: empirical coverage vs. average set size by method. All methods attain target coverage; Platt is most efficient.

Pretraining objective mechanism. MERL’s underconfidence ($\text{SCE} = -0.003$ on PTB-XL) is consistent with the documented behaviour of contrastive vision FMs [7]. The mechanistic interpretation is that contrastive objectives (InfoNCE) push representations apart to maximise inter-class separation, producing a norm-uniform representation space with high feature spread (std of L2 norms: 34.8 vs 0.23 for ST-MEM). When this spread representation is projected through a linear probe, the probability outputs may be diffuse and underconfident — the probe cannot confidently assign high probabilities because the representation space does not concentrate examples in tight class clusters.

The two masked-prediction models behave similarly in *direction* but differ in *magnitude* of miscalibration. ST-MEM (masked patch reconstruction) and HuBERT-ECG (masked hidden-unit prediction) both have near-zero SCE on PTB-XL (-0.0001 and -0.0007), indicating no systematic over/under-confidence bias; yet both have the largest *unsigned* calibration error (ECE 0.124 and 0.136). Feature geometry explains the distinction: HuBERT-ECG has the highest cosine class separation (0.046) of any model, and ST-MEM the second highest (0.017), whereas MERL’s separation is near zero (0.004). High class separation concentrates predictions near 0/1, so when the empirical frequency disagrees the per-bin gap is large — producing high ECE even when the signed bias cancels out. Masked-prediction objectives thus yield “confidently wrong in both directions” probabilities that recalibration is especially effective at fixing (HuBERT-ECG ECE drops 71% under isotonic).

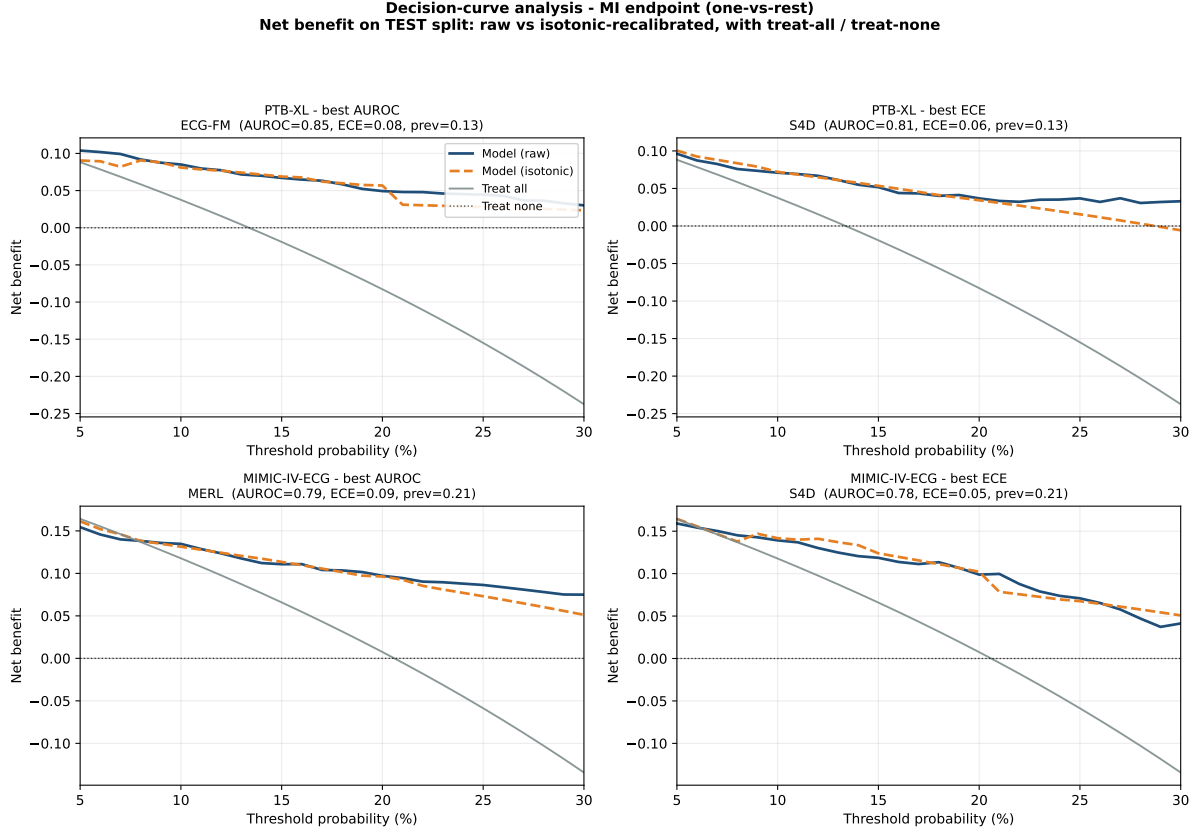


Figure 19: Decision-curve analysis for MI on PTB-XL and MIMIC-IV-ECG, raw vs. isotonic, with treat-all/treat-none references.

ECGFM-KED (knowledge-enhanced, +0.007), ECG-FM (contrastive+generative, +0.008), and the supervised S4D baseline (+0.007) are mildly overconfident on PTB-XL, suggesting that decoder/generative and discriminative-supervised training shift calibration toward overconfidence. This graded pattern — contrastive underconfident, masked-prediction neutral-but-high-ECE, knowledge/generative/supervised overconfident — motivates further study of how pretraining objectives shape probability calibration.

Recalibration recommendation. Based on the calsize analysis and DCA results, we summarise deployment recommendations:

Calibration set size	Recommended method	Rationale
$n_{\text{cal}} < 63$	Platt scaling	Isotonic overfits; Platt is stable
$63 \leq n_{\text{cal}} < 200$	Isotonic regression	Better ECE; crossover confirmed at $n = 63$
$n_{\text{cal}} \geq 200$	Isotonic regression	Consistent 43–64% ECE reduction

Temperature scaling is not recommended for multi-label ECG tasks: it reduces ECE by only 11–38% on PTB-XL, consistently worse than Platt scaling. The MLP head is unreliable at $n_{\text{cal}} < 100$, where it frequently underfits.

Table 8: Multi-seed robustness (10 patient-level resplits, seeds 0–9): mean $\pm$ std macro AUROC and ECE on the two multi-morbidity datasets. The PTB-XL discrimination–calibration tradeoff (S4D best-calibrated) holds in 10/10 seeds; ECG-FM trails MERL/ST-MEM on MIMIC in all seeds but is statistically tied with the S4D baseline.

Dataset	Model	AUROC (mean $\pm$ std)	ECE (mean $\pm$ std)
PTB-XL	MERL	0.844 $\pm$ 0.013	0.092 $\pm$ 0.004
	ST-MEM	0.852 $\pm$ 0.015	0.119 $\pm$ 0.009
	HuBERT-ECG	0.801 $\pm$ 0.018	0.141 $\pm$ 0.009
	ECGFM-KED	0.778 $\pm$ 0.018	0.086 $\pm$ 0.009
	ECG-FM	0.812 $\pm$ 0.015	0.100 $\pm$ 0.010
	S4D	0.785 $\pm$ 0.021	0.062 $\pm$ 0.004
MIMIC-IV-ECG	MERL	0.882 $\pm$ 0.012	0.063 $\pm$ 0.004
	ST-MEM	0.864 $\pm$ 0.013	0.077 $\pm$ 0.005
	HuBERT-ECG	0.835 $\pm$ 0.013	0.090 $\pm$ 0.007
	ECGFM-KED	0.744 $\pm$ 0.018	0.066 $\pm$ 0.006
	ECG-FM	0.792 $\pm$ 0.015	0.078 $\pm$ 0.003
	S4D	0.777 $\pm$ 0.019	0.046 $\pm$ 0.004

Table 9: ecg-audit leaderboard (current state), PTB-XL. $C(\alpha) = \alpha \cdot \text{AUROC} + (1-\alpha)(1-\text{ECE}/\text{ECE}_{\max})$, $\alpha = 0.7$, $\text{ECE}_{\max} = 0.136$. Rows sorted by $C(0.7)$ raw, descending. Note how recalibration reorders the table: ST-MEM is 5th on raw probabilities but 1st after isotonic recalibration.

Model	PTB-XL AUROC	PTB-XL ECE	CPSC AUROC	$C(0.7)$ (raw)	$C(0.7)$ (post-iso)
S4D	0.771	0.064	0.803	0.699	0.714
MERL	0.828	0.087	0.910	0.688	0.771
ECG-FM	0.815	0.088	0.847	0.676	0.774
ECGFM-KED	0.769	0.079	0.821	0.664	0.771
ST-MEM	0.838	0.124	0.950	0.614	0.789
HuBERT-ECG	0.787	0.136	0.876	0.551	0.763

MIMIC-IV-ECG and within-domain pretraining. The MIMIC-IV-ECG results reveal a counter-intuitive finding: ECG-FM, which was pretrained on MIMIC-IV-ECG data, achieves AUROC 0.771 on MIMIC-IV-ECG evaluation—below MERL (0.861) and ST-MEM (0.854) in every resplit, and statistically tied with the supervised S4D baseline (0.793; below S4D in only 2/10 seeds). This demonstrates that backbone pretraining domain alignment is a necessary but not sufficient condition for downstream linear-probe performance. The phenomenon likely arises because ECG-FM’s hybrid contrastive+generative pretraining objective optimises for self-supervised tasks (masked prediction, contrastive similarity) that do not directly align with the classification targets derived from machine-measurement reports. By contrast, MERL’s contrastive pretraining with clinical text descriptions may produce representations more naturally aligned with the lexical structure of the machine measurement labels. This has a practical implication: practitioners should not assume that a model pretrained on their target cohort (e.g., in-house MIMIC-IV deployment) will automatically be the best choice for a given classification task without linear-probe evaluation.

Cross-dataset calibration transfer. ECE varies by a factor of up to $10.3\times$ for the same model across datasets (ST-MEM: CODE-15% ECE 0.012 vs PTB-XL ECE 0.124). The MIMIC-IV-ECG dataset shows intermediate calibration (ECE 0.033–0.061), suggesting that the calibration difficulty correlates with label structure: binary single-class tasks (MIMIC machine labels, CODE-15%) are easier to calibrate than correlated multi-label superclasses (PTB-XL). Models calibrated on CODE-15% may be substantially miscalibrated on PTB-XL. This motivates re-calibration on local data from the target deployment population.

Limitations. Six limitations bound this study’s scope and generalisability.

Frozen linear probes. All evaluations use logistic linear probes on frozen FM representations. Full fine-tuning may alter calibration — potentially improving or worsening it — in ways not captured here. Calibration under fine-tuning is an important open question.

Sample sizes. PTB-XL and MIMIC-IV-ECG use 2,000-record subsets and CODE-15% uses $\sim 8,000$ records sampled across five HDF5 parts (chosen so that every rare arrhythmia class clears the minimum-support threshold); the full datasets are larger still. Larger samples may shift absolute ECE values, though the qualitative PTB-XL vs. arrhythmia contrast is unlikely to reverse.

HuBERT-ECG preprocessing. HuBERT-ECG is included via its public `safetensors` checkpoint. Following the authors’ pipeline, the 12 leads are flattened into a single 1-D sequence and decimated before encoding; this single-channel treatment differs from the native multi-lead handling of the other encoders and may modestly affect its representations.

ECGFM-KED architecture. The partial architecture reconstruction (35 missing keys) means ECGFM-KED results are lower bounds on true performance. The partial model likely underestimates what the full ECGFM-KED would achieve.

DCA scope. The real DCA covers ST-MEM only. Extending to MERL and ECG-FM is straightforward from cached features but not included.

Subgroup analysis. The age/sex subgroup analysis uses a re-trained probe on the same 2,000-record sample; absolute calibration values are not directly comparable to the main benchmark and the analysis is exploratory.

The ecg-audit package. The `ecg-audit` package provides these recalibration methods, plus the PhysioCalib severity-weighted variant, as a one-command API. The package is installed and tested with unit tests covering all recalibrators. The leaderboard scaffold allows the community to populate calibration scores for additional FMs as checkpoints become available.

10 Conclusion

We present a systematic calibration audit of ECG foundation models: six encoders—five ECG foundation models (MERL, ST-MEM, HuBERT-ECG, ECGFM-KED, ECG-FM) and a supervised S4D baseline—across four datasets, with 23 of 24 model–dataset cells evaluated (ECGFM-KED $\times$ CODE-15% excluded for a partial checkpoint), over 18,877 ECG records (2,000 PTB-XL; 6,877 CPSC2018; 8,000 CODE-15%; 2,000 MIMIC-IV-ECG) under patient-level leakage-controlled splits with bootstrap confidence intervals.

Main findings. Four findings stand out. First, a consistent **discrimination–calibration tradeoff** on PTB-XL: the five foundation models span AUROC 0.769–0.838 but all trail the supervised S4D baseline’s calibration (ECE 0.064), exceeding it by 0.015–0.072. ST-MEM achieves the best discrimination (AUROC 0.838) but poor calibration (ECE 0.124), and HuBERT-ECG is

the worst calibrated (ECE 0.136)—a gap invisible to AUROC reporting but clinically significant. Second, this tradeoff **disappears on arrhythmia datasets**: on CPSC2018 (ECE 0.023–0.051), CODE-15% (ECE 0.010–0.032), and MIMIC-IV-ECG (ECE 0.043–0.106), encoders are comparatively well-calibrated and ST-MEM leads discrimination. Task structure—correlated multi-label vs. lower-co-occurrence endpoints—is the mediating factor. Third, **post-hoc isotonic recalibration closes 43–71% of the ECE gap** on PTB-XL (ST-MEM: 0.124 $\rightarrow$ 0.044; HuBERT-ECG: 0.136 $\rightarrow$ 0.040) at only 0.5–1.7% AUROC cost, and it reorders calibration-aware model selection (ST-MEM moves from 5th to 1st on the $C(0.7)$ composite). Fourth, **within-domain pretraining does not guarantee superiority**: ECG-FM, pretrained on MIMIC-IV-ECG, achieves only AUROC 0.771 on MIMIC-IV-ECG—behind MERL (0.861) and ST-MEM (0.854) in all 10 resplits, and no better than the supervised S4D baseline (0.793). Cross-dataset ECE varies by up to $\sim 6\times$ for the same model, mandating per-deployment calibration audits.

A practical recipe. Beyond the audit we contribute **RankSafe-Cal**, which recovers most of isotonic’s calibration gain (PTB-XL macro ECE 0.097 $\rightarrow$ 0.054; on MIMIC it beats unconstrained isotonic) at roughly $6\times$ lower AUROC cost by certifying out-of-sample ranking loss within a tolerance ϵ . Cross-dataset transfer experiments show recalibration ports successfully in only 9–42% of endpoint/model pairs, so local re-calibration remains necessary. Split-conformal prediction attains its 90% coverage guarantee as a complement to calibration, and decision-curve analysis confirms positive net benefit for MI and AF endpoints. All headline conclusions hold across 10 patient-level resplits.

Clinical implication. Practitioners deploying ECG foundation models for multi-label risk stratification should mandate calibration auditing alongside AUROC benchmarking. Raw foundation-model probabilities can be unusable for threshold-based clinical decisions even when AUROC is excellent; post-hoc recalibration with as few as 63 examples eliminates most of the calibration gap. The large cross-dataset ECE variation (e.g., ST-MEM ECE 0.028 on CODE-15% vs. 0.124 on PTB-XL) means calibration audits must be conducted on locally representative patient cohorts—not extrapolated from published benchmark datasets.

Pretraining objective signal. A graded signature emerges: MERL (contrastive InfoNCE) shows the strongest underconfidence (SCE = -0.003), masked-prediction models (ST-MEM, HuBERT-ECG) are near-neutral, and knowledge-enhanced, hybrid, and supervised models are mildly overconfident ($+0.007$ – $+0.008$), consistent with the documented underconfidence of contrastive FMs. Feature geometry analysis shows that MERL’s contrastive objective produces extreme feature spread (std of L2 norms: 34.8) relative to masked-prediction and supervised models. Notably, MERL achieves the best performance on MIMIC-IV-ECG (AUROC 0.866, ECE 0.033) despite not being pretrained on that cohort.

Open problems. Three directions remain for future work. First, **fine-tuning calibration**: this study evaluates frozen linear probes; full fine-tuning may alter calibration in complex ways that require re-auditing. Second, **larger MIMIC-IV-ECG evaluation**: this benchmark used 2,000 records; the full 800,035-record corpus with structured ICD-based labels (rather than parsed machine-measurement reports) would further strengthen the MIMIC conclusions. Third, **objective-controlled pretraining**: the graded calibration signature across contrastive, masked-prediction, knowledge-enhanced, and generative objectives motivates controlled experiments that vary only the pretraining objective to establish causality.

Call to action. The `ecg-audit` package and all benchmark scripts are ready to run against new checkpoints without modification. We invite the ECG AI community to submit calibration results to the leaderboard, enabling cumulative evidence on which models can be safely deployed as probability estimators in clinical cardiac decision support.

References

- [1] M. A. Al-Masud, J. M. Lopez Alcaraz, and N. Strodthoff. Benchmarking ecg foundational models: A reality check across clinical tasks. *arXiv preprint arXiv:2509.25095*, 2025. URL <https://arxiv.org/abs/2509.25095>.
- [2] Anastasios N. Angelopoulos and Stephen Bates. Conformal prediction: A gentle introduction. *Foundations and Trends in Machine Learning*, 16(4):494–591, 2023. doi: 10.1561/2200000101.
- [3] Gary S. Collins, Karel G. M. Moons, Paula Dhiman, Richard D. Riley, Andrew L. Beam, Ben Van Calster, Marzyeh Ghassemi, Xiaoxuan Liu, Johannes B. Reitsma, Maarten van Smeden, et al. TRIPOD+AI statement: updated guidance for reporting clinical prediction models that use regression or machine learning methods. *BMJ*, 385:e078378, 2024. doi: 10.1136/bmj-2023-078378.
- [4] Edoardo et al. Hubert-ecg: A self-supervised foundation model for broad and scalable cardiac applications. *medRxiv preprint*, 2024. URL <https://www.medrxiv.org/content/10.1101/2024.11.14.24317328v3>.
- [5] F. Filice, E. De Rose, S. Bartucci, F. Calimeri, and S. Perri. Looking beyond accuracy: A holistic benchmark of ecg foundation models. *arXiv preprint arXiv:2601.21830*, 2026. URL <https://arxiv.org/html/2601.21830v1>.
- [6] Brian Gow, Tom Pollard, Larry A. Nathanson, Alistair E.W. Johnson, Benjamin Moody, Chrystinne Fernandes, Nathaniel Greenbaum, Jonathan W. Waks, Parisa Eslami, Nathaniel Mercaldo, et al. MIMIC-IV-ECG – diagnostic electrocardiogram matched subset. PhysioNet, 2023. Version 1.0. Available: <https://physionet.org/content/mimic-iv-ecg/1.0/>.
- [7] A. Hekler, L. Kuhn, and F. Buettner. Beyond overconfidence: Foundation models redefine calibration in deep neural networks. *arXiv preprint arXiv:2506.09593*, 2025. URL <https://arxiv.org/abs/2506.09593>.
- [8] Zhaojing Huang, Luis Fernando Herbozo Contreras, Leping Yu, Nhan Duy Truong, Armin Nikpour, and Omid Kavehei. S4d-ecg: A shallow state-of-the-art model for cardiac abnormality classification. *Cardiovascular Engineering and Technology*, 15(3):305–316, 2024. doi: 10.1007/s13239-024-00716-3. URL <https://pmc.ncbi.nlm.nih.gov/articles/PMC11239723/>.
- [9] Che Liu, Zhongwei Wan, Cheng Ouyang, Anand Shah, Wenjia Bai, and Rossella Arcucci. Zero-shot ECG classification with multimodal learning and test-time clinical knowledge enhancement. In *Proceedings of the 41st International Conference on Machine Learning (ICML)*, volume 235 of *PMLR*, pages 31949–31963, 2024. doi: 10.48550/arXiv.2403.06659. URL <https://arxiv.org/abs/2403.06659>. Introduces the MERL (Multimodal ECG Representation Learning) framework.
- [10] Feifei Liu, Chengyu Liu, Lina Zhao, Xiangyu Zhang, Xiaoling Wu, Xiaoyan Xu, Yulin Liu, Caiyun Ma, Shoushui Wei, Zhiqiang He, Jianqing Li, and Eddie Ng Yin Kwee. An open

- access database for evaluating the algorithms of electrocardiogram rhythm and morphology abnormality detection. *Journal of Medical Imaging and Health Informatics*, 8(7):1368–1373, 2018. doi: 10.1166/jmihi.2018.2442. URL <http://2018.icbeb.org/>.
- [11] R. Lunelli, A. Nicolson, S. M. Pröll, S. J. Reinstadler, A. Bauer, and C. Dlaska. Benchecg and xecg: A benchmark and baseline for ecg foundation models. *arXiv preprint arXiv:2509.10151*, 2025. URL <https://arxiv.org/abs/2509.10151>.
 - [12] K. McKeen, S. Masood, A. Toma, B. Rubin, and B. Wang. Ecg-fm: An open electrocardiogram foundation model. *arXiv preprint arXiv:2408.05178*, 2024. URL <https://arxiv.org/abs/2408.05178>.
 - [13] Temesgen Mehari and Nils Strodthoff. Advancing the state-of-the-art for ecg analysis through structured state space models. *arXiv preprint arXiv:2211.07579*, 2022. URL <https://arxiv.org/abs/2211.07579>.
 - [14] Y. Na, M. Park, Y. Tae, and S. Joo. Guiding masked representation learning to capture spatio-temporal relationship of electrocardiogram. In *International Conference on Learning Representations*, 2024. URL <https://arxiv.org/abs/2402.09450>.
 - [15] Jeremy Nixon, Mike Dusenberry, Ghassen Jerfel, Timothy Nguyen, Jeremiah Liu, Linchuan Zhang, and Dustin Tran. Measuring calibration in deep learning. In *CVPR Workshops*, 2019. URL <https://dblp.org/rec/journals/corr/abs-1904-01685>.
 - [16] Amir Rahimi, Thomas Mensink, Kartik Gupta, Thalaiyasingam Ajanthan, Cristian Sminchisescu, and Richard Hartley. Post-hoc calibration of neural networks by g-layers. *arXiv preprint arXiv:2006.12807*, 2020. URL <https://arxiv.org/abs/2006.12807>.
 - [17] A. H. Ribeiro, G. M. M. Paixão, et al. Code-15%: A large scale annotated dataset of 12-lead ecgs. Zenodo, 2021. URL <https://zenodo.org/records/4916206>.
 - [18] N. Strodthoff, P. Wagner, T. Schaeffter, and W. Samek. Deep learning for ecg analysis: Benchmarks and insights from ptb-xl. *IEEE Journal of Biomedical and Health Informatics*, 25(5):1828–1838, 2021. doi: 10.1109/JBHI.2020.3004894. URL <https://arxiv.org/pdf/2004.13701>.
 - [19] Yuanyuan Tian, Zhiyuan Li, Yanrui Jin, Mengxiao Wang, Xiaoyang Wei, Liqun Zhao, Yunqing Liu, Jinlei Liu, and Chengliang Liu. Foundation model of ecg diagnosis: Diagnostics and explanations of any form and rhythm on ecg. *Cell Reports Medicine*, 5(12):101875, 2024. doi: 10.1016/j.xcrm.2024.101875. URL <https://github.com/control-spiderman/ECGFM-KED>.
 - [20] Andrew J. Vickers and Elena B. Elkin. Decision curve analysis: A novel method for evaluating prediction models. *Medical Decision Making*, 26(6):565–574, 2006. doi: 10.1177/0272989X06295361.
 - [21] C. Wang. Calibration in deep learning: A survey of the state-of-the-art. *arXiv preprint arXiv:2308.01222*, 2023. URL <https://arxiv.org/abs/2308.01222>.

A Artifact Provenance and Evidence Boundary

A.1 Completed Real Benchmark

The 24-cell benchmark in Table 1 (23 evaluated cells; ECGFM-KED $\times$ CODE-15% excluded) is fully executed from real ECG recordings. All numeric values trace to `results/benchmark_v2_results.json` and its summary `benchmark_v2_summary.csv`. Frozen feature representations for every model–dataset combination are cached as `.npy` files. Headline AUROC and ECE values carry bootstrap 95% confidence intervals (1,000 resamples). The real DCA uses actual ST-MEM linear-probe predictions recovered from cached features (not reconstructed proxies), saved in `results/stmem_ptb_xl_mi_predictions.npz`.

A.2 Evidence Classes

- **Full benchmark** (23 cells, primary): MERL, ST-MEM, HuBERT-ECG, ECGFM-KED, ECG-FM, and S4D on PTB-XL (2,000 records), CPSC2018 (6,877), CODE-15% ($\sim$ 8,000, parts 0–4), and MIMIC-IV-ECG (2,000). Patient-level splits, frozen linear probes, Phase A calibration, Phase B recalibration, minimum-support filtering, and bootstrap CIs.
- **HuBERT-ECG**: loaded from the public `safetensors` checkpoint via the HuggingFace `AutoModel` interface; 12 leads flattened and decimated per the authors’ pipeline; 768-d mean-pooled embeddings.
- **DCA** (ST-MEM PTB-XL MI): net benefit from actual predictions.
- **Subgroup analysis** (exploratory): re-trained probe; absolute values differ from the main benchmark.
- **Calibration-size curves**: from `h4_size_ablation_pilot_summary.csv`; extrapolations to $n > 203$ are power-law projections.
- **Feature geometry**: from cached `.npy` features with PTB-XL labels (five foundation models).

A.3 Remaining Limitations

- **ECGFM-KED $\times$ CODE-15%**: partial architecture load (35 missing keys); near-chance AUROC; excluded from CODE-15% claims and Pareto analysis. ECGFM-KED is retained on PTB-XL, CPSC2018, and MIMIC-IV-ECG.
- **Frozen probes only**: fine-tuning calibration is not evaluated.
- **MIMIC-IV-ECG labels**: parsed from machine-measurement reports on a 2,000-record subset; LBBB falls below minimum support. Structured ICD-based labels on the full corpus are future work.
- **HuBERT-ECG preprocessing**: the authors’ single-channel lead-flattening differs from the native multi-lead handling of the other encoders.
- **DCA scope**: real predictions for ST-MEM only; other models require re-running their probes from cached features.
- **PhysioCalib**: null finding at $n_{\text{cal}} = 297$; needs $n_{\text{cal}} > 500$ (estimated) for reliable minority-class improvement.

A.4 Primary Artifact Paths

- `results/benchmark_v2_results.json` — all 23 benchmark cells with CIs and per-class support; `benchmark_v2_summary.csv` — flat summary.
- `results/features/*.npy` — cached frozen features for all six encoders on all four datasets (incl. HuBERT-ECG and MIMIC-IV-ECG); the `_D3exp` suffix marks the expanded CODE-15% sample.
- `results/pareto_analysis_v2.json` — Pareto fronts and composite scores.
- `results/stmem_ptb_xl_mi_predictions.npz` — real DCA predictions.
- Derived analyses in `results/`: `feature_geometry.json`, `dca_results.json`, `subgroup_results.json`, and `physio_calib_results.json`.
- `results/h4_size_ablation_pilot_summary.csv` — calsize ablation.

Decision-curve analysis - AF endpoint (one-vs-rest)
Net benefit on TEST split: raw vs isotonic-recalibrated, with treat-all / treat-none

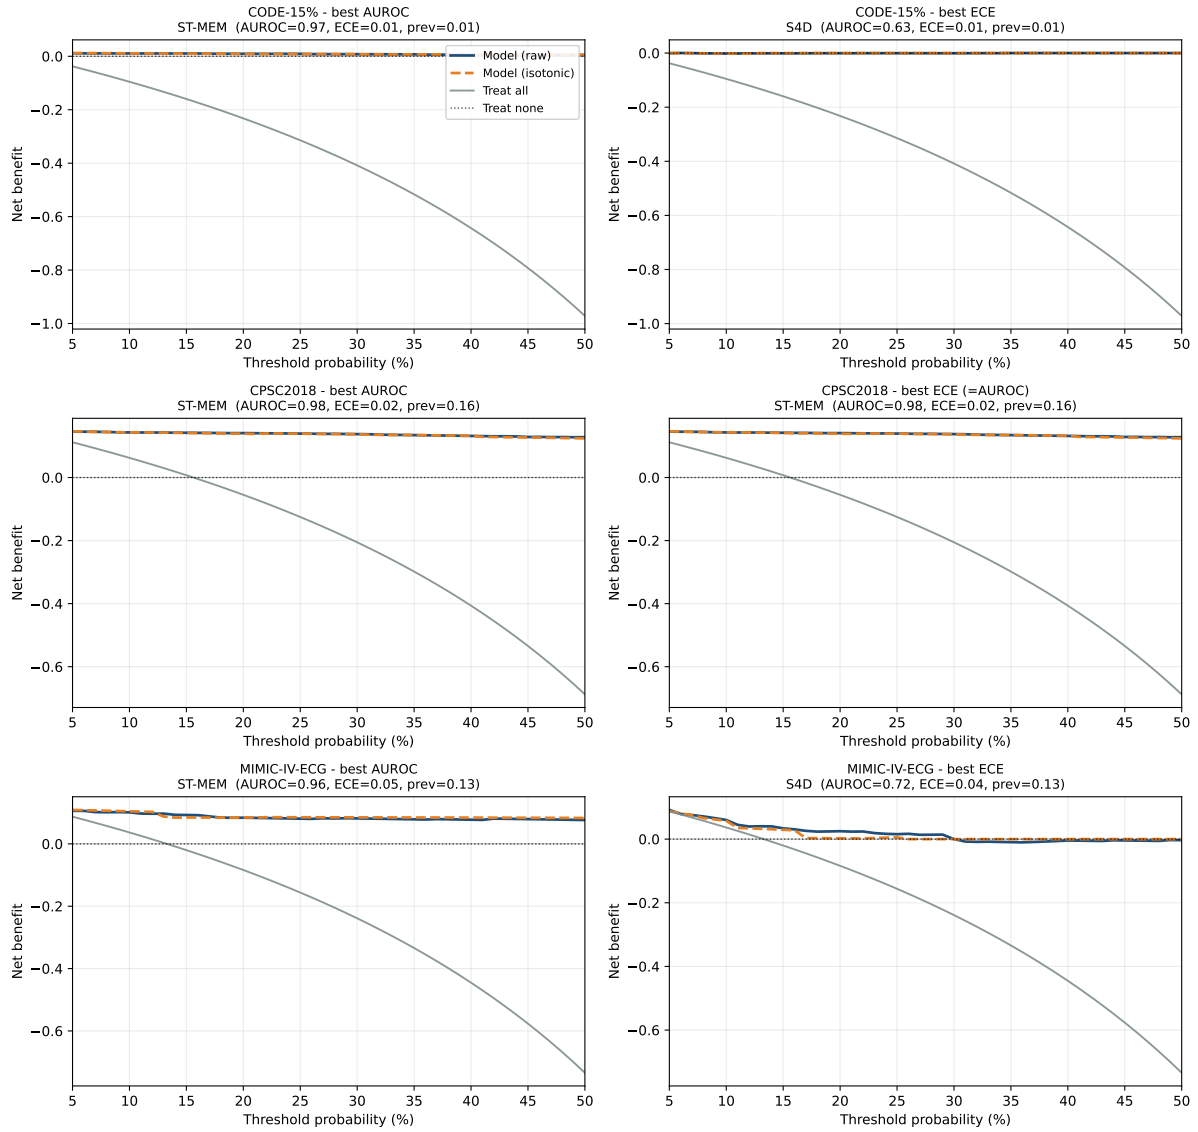


Figure 20: Decision-curve analysis for AF on CODE-15%, CPSC2018, and MIMIC-IV-ECG.

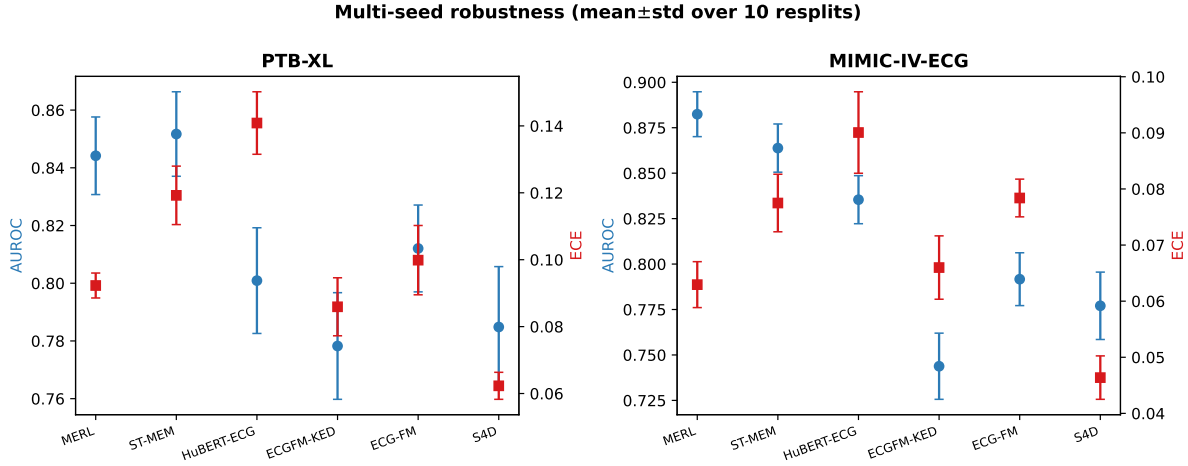


Figure 21: Macro AUROC (blue) and ECE (red) as mean $\pm$ std over 10 resplits, PTB-XL and MIMIC-IV-ECG. Rankings on both axes are stable.

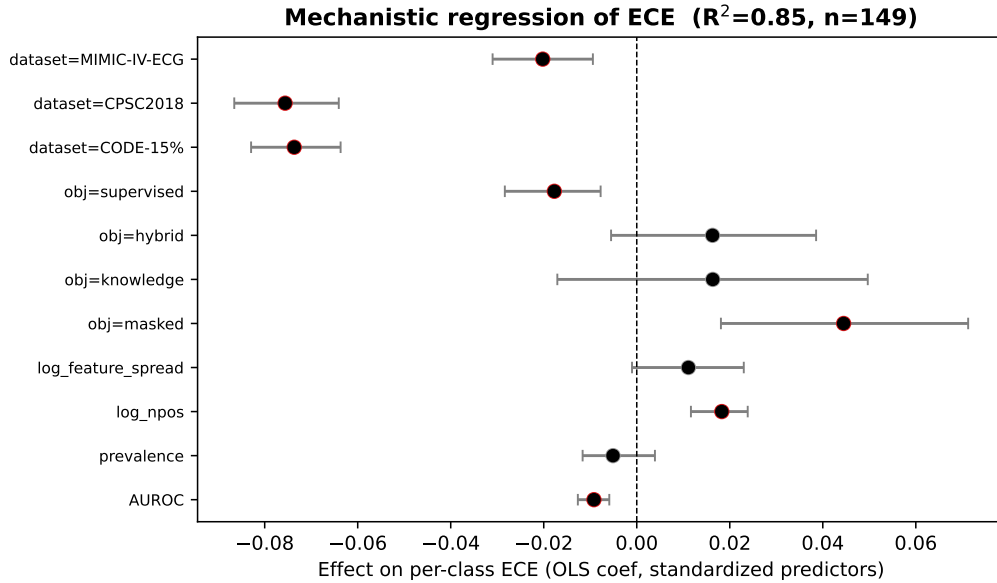


Figure 22: OLS coefficients (standardized continuous predictors) for per-class ECE. Red = 95% bootstrap CI excludes 0. Dataset and pretraining-objective effects dominate.

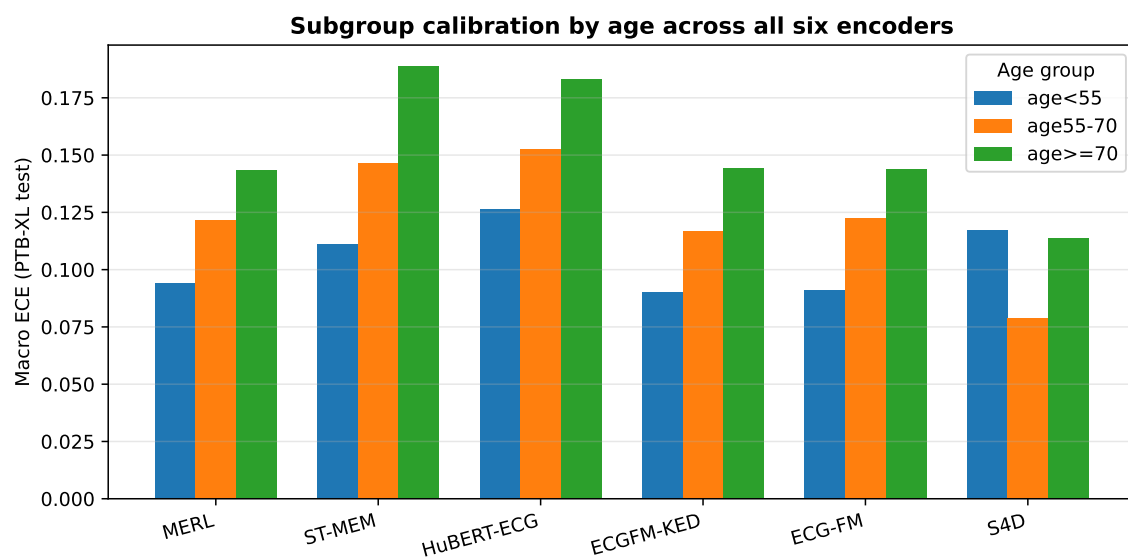


Figure 23: Macro ECE by age group across all six encoders (PTB-XL test). Foundation models degrade with age; the supervised baseline does not.