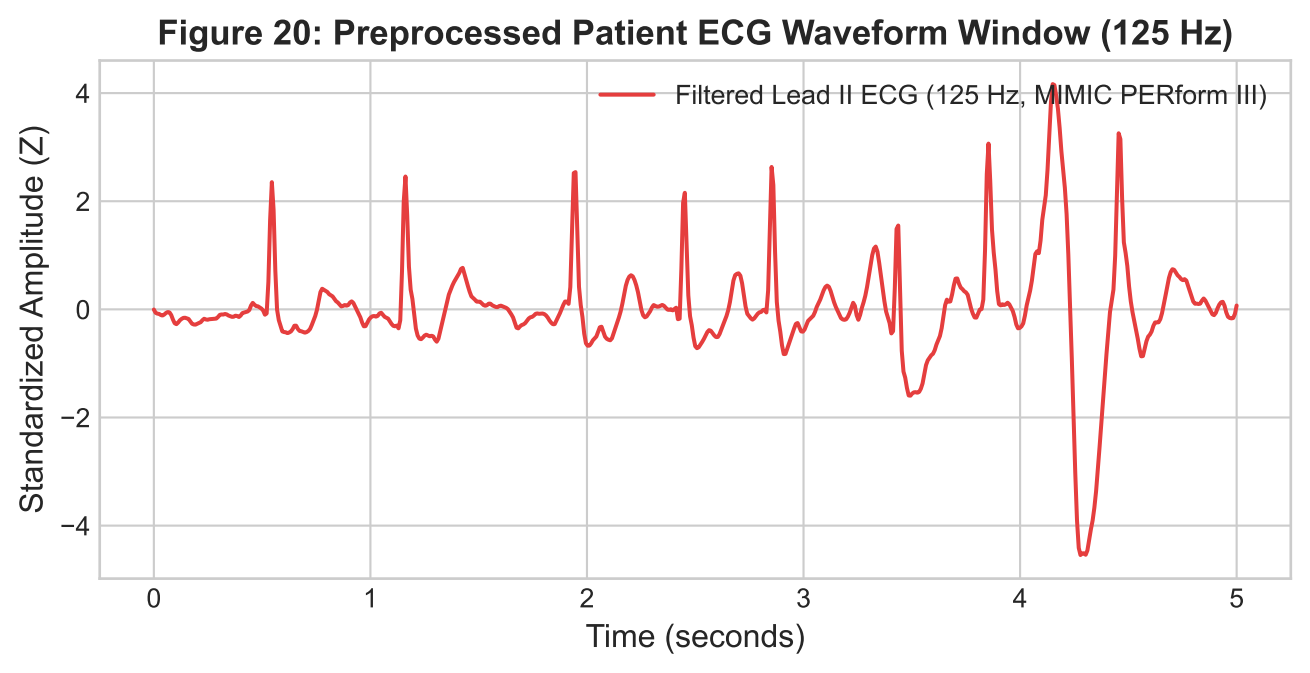
Figure 20: Preprocessed Patient ECG Waveform Window (125 Hz)
Filtered Lead II ECG (125 Hz, MIMIC PERform III)
Standardized Amplitude (Z)
4
2
0
−2
−4
0
1
2
3
4
5
Time (seconds)