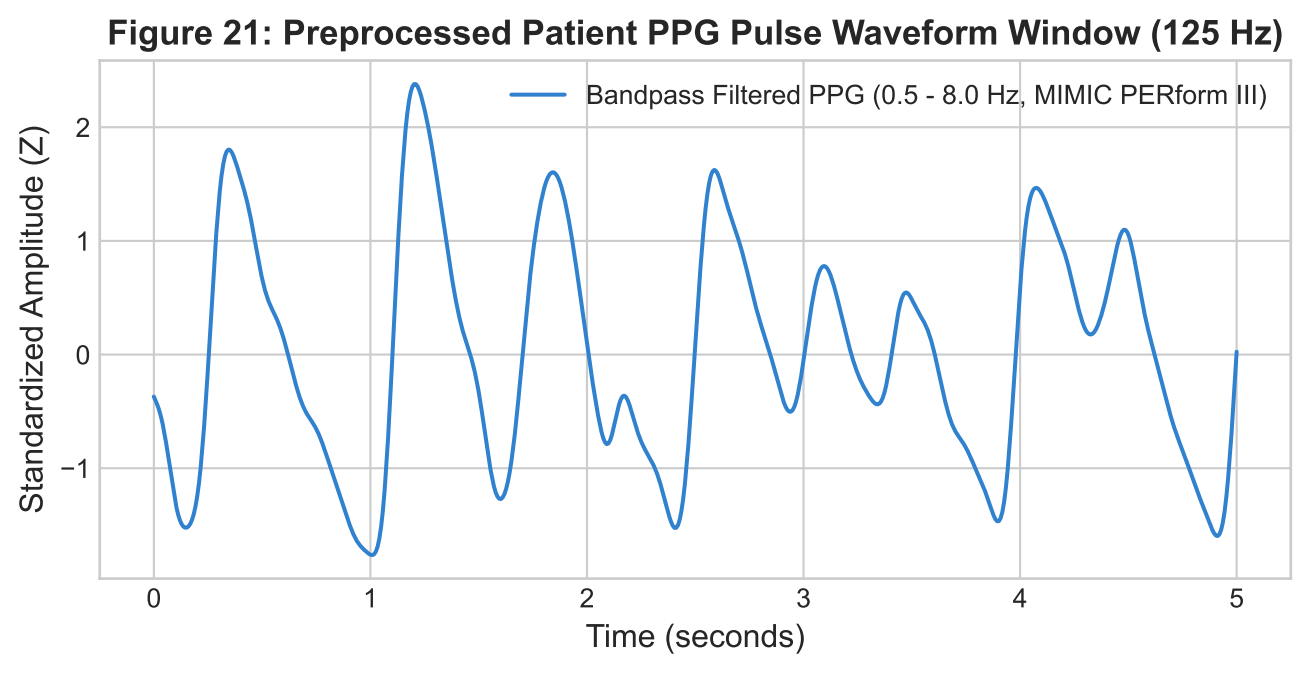
Figure 21: Preprocessed Patient PPG Pulse Waveform Window (125 Hz)
Bandpass Filtered PPG (0.5 - 8.0 Hz, MIMIC PERform III)
Standardized Amplitude (Z)
2
1
0
−1
0
1
2
3
4
5
Time (seconds)