



Filename: 12.plux

Acquisition author: Advanced

Analysis author:

Company name: Sensofar S.L.

Date: 2023-08-11 00:48:32


Analysis Software Version: 1.8.0.0

Acquisition

Topography: 1349 x 1853 px
Operator: Advanced
Area: 0.87 x 1.19 mm
Date: 2023-08-02
Pixel Size: 0.64 µm/pixel
Time: 11:27:56
Measure type: Topography
Technique: Confocal
Algorithm: Continuous Confocal
Z SCAN: 500 µm
Threshold: 0.10%
Measured: 47.84%

Light: 8.00%
Ring light: 0.00%
Acq. time: 01:10
Type: NonContacting
Manufacturer: Sensofar
Model: S neox
SN: unknown
Version: SensoSCAN 6
Objective: EPI 20X
Calib. date: unknown
Reference: 225MUE10200
Magnification: 20.00

Visualization

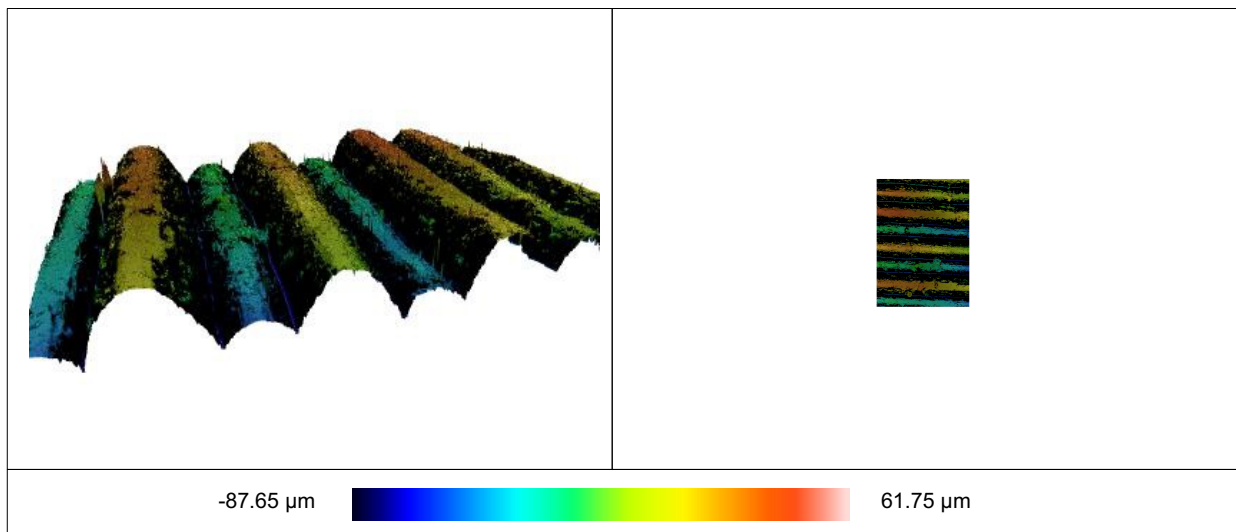

ISO 25178 / Height

Sa 21.943 µm
Sku 1.9541
Smean -13.360 µm
Sp 75.105 µm

Sq 25.228 µm
Ssk -0.0898
Sv 74.285 µm
Sz 149.39 µm

Comment

-