SureSet™
Loop IV Securement Device (Pediatric)

Instructions for Use

Manufactured for:
Alera Medtech LLC
77 Rowe Street, Suite 2C
Auburndale
MA 02466-1532
USA

To report any quality issues or concerns, please contact us at:

+1 (888) 70ALERA

+1 (888) 702-5372

customerservice@aleramedtech.com

www.suresetsecure.com

IMPORTANT: Carefully read and understand all instructions, indications, warnings and precautions and directions for use prior to using the SureSet™ Securement device. Failure to do so could result in compromised patient safety, patient complications and/or insufficient treatment.

Trademarks and Copyright
SureSet™ is a trademark of Alera Medtech™
© Alera Medtech, LLC. 2026. All rights reserved.
Patent US 2025/0065034 A1

Visit our website to learn more

Visit our training video to learn more

SureSet™
Loop IV Securement Device (Pediatric)

Intended use

The Device is intended to secure a range of compatible peripheral IV catheters to reduce catheter movement and help prevent unintentional dislodgement.
Tubing – 16G to 30G

Safety considerations

Single use only.
Discard if package is damaged.

Training Alera offers SureSet Loop IV training for users prior to use. Use the QR code on page 1 to view the training.

Familiarity with IV procedures

Users should be familiar with IV procedures and techniques for vascular access device care and management.

Key usage points

- Prepare the skin: cleanse skin with antiseptic wipe and allow to dry completely.
- Affix the device as described on page 4.
- To access the IV tubing, place finger under clasp and lift to open the cover of the SureSet device.
- Remove any residue of the dressing pad adhesive with alcohol after removing the device.
- Remove the device as described on page 5.
- Discard after use.

Device overview

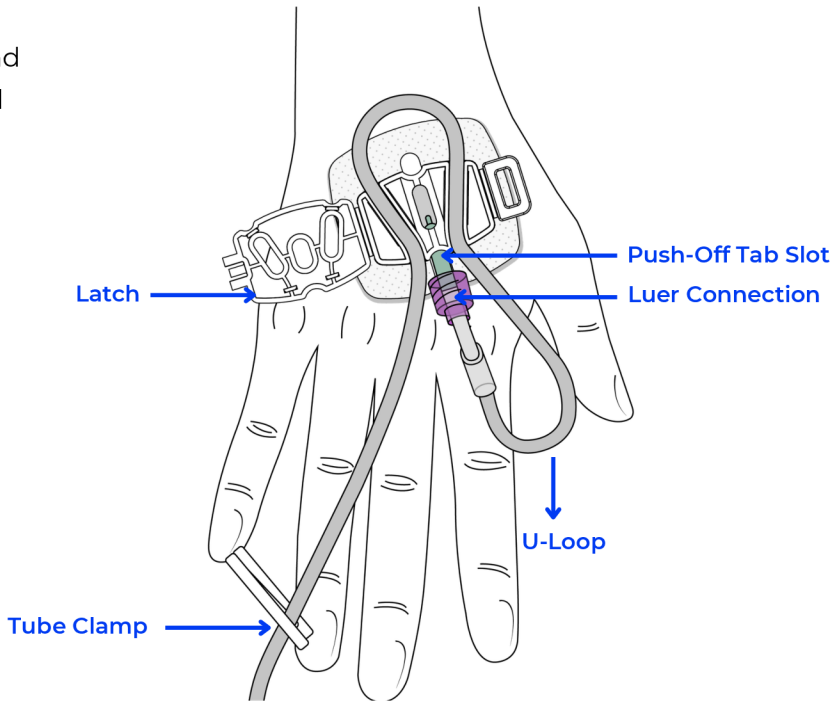

This section contains important safety information. Please read and understand all warnings, precautions, and instructions for use prior to using the SureSet Loop IV Securement Device.

⚠ Warnings

- Do not use the device where loss of adhesive could occur, such as non-adherent skin or confused patient.
- Use aseptic technique for application and removal of the device. In case of device loosening or malfunction, the device should be removed and replaced.
- In case of device loosening or malfunction, the device should be removed and replaced.

⚠ Precautions

- Read all package insert warnings and instructions prior to use.
- The device and the surrounding area should be routinely inspected.
- Minimize catheter or tubing manipulation during application and removal of the device.
- Remove any oil and moisturizer from the targeted skin area before application.
- Respect infection control guidelines during application and removal of the device, wash hands before use.
- This is a single use device. Do not reuse. If reused, the adhesive may not maintain its performance, causing the device to loosen from the skin.

Incidents should be reported to the manufacturer.

The following symbols may appear in this IFU, on the SureSet device and on the SureSet packaging. Some of the symbols represent standards and compliances associated with the SureSet Loop IV Securement Device and its use.

Warning	Keep dry	Quantity
Caution	Single use	Consult instructions for use
Date of Manufacture	Do not use if package is damaged	Manufacturer
REF Catalog Number	LOT Lot Number	STERILE EO Device is sterile

Instructions for Use

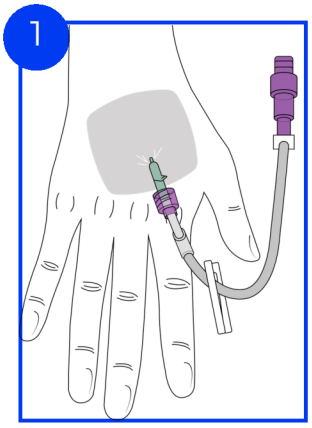

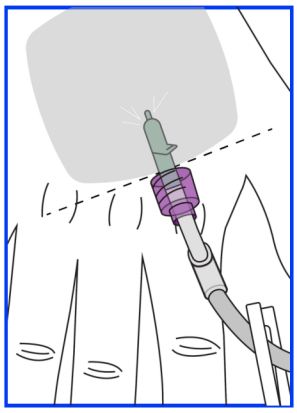

Place the protective dressing over the IV catheter hub. Do not cover the Luer connection with the protective dressing.

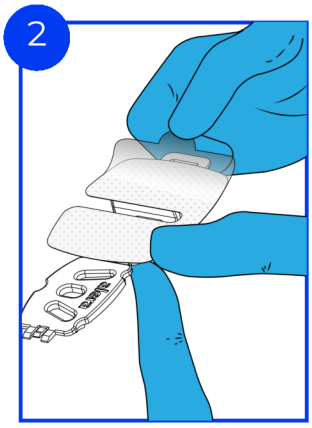

Peel off the adhesive cover to reveal adhesive strip on underside of SureSet.

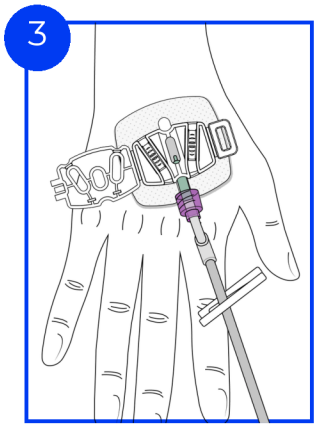

Place the device over the protective dressing, ensuring it adheres securely.

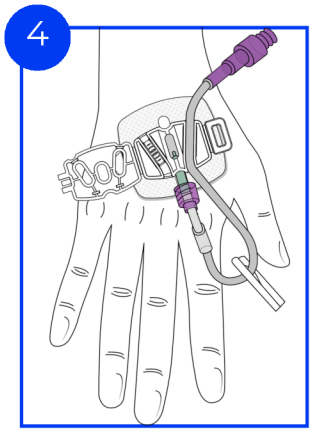

Press and secure tubing into the side channel. (supported tubing size - 16G to 30G)

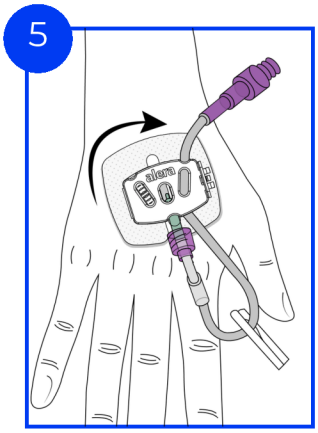

Close the device cover. Make sure it closes securely.

Additional Configurations & Removal

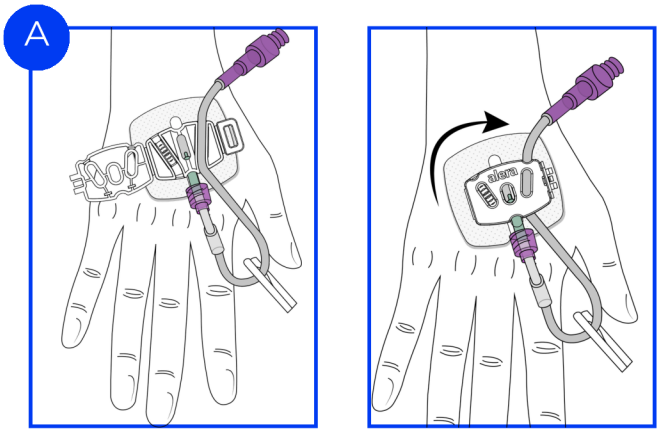

Configuration A

Standard configuration as shown on previous page.

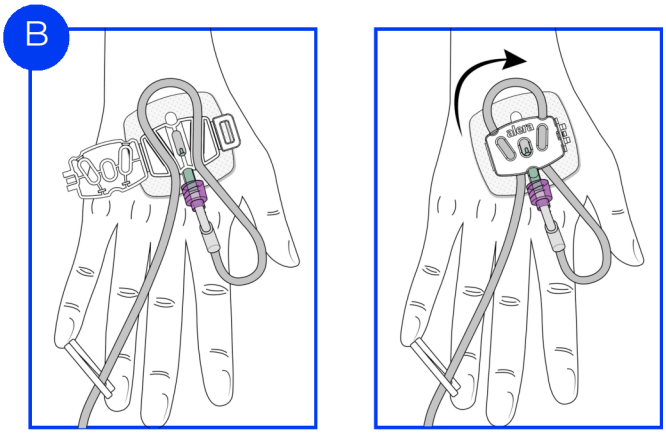

Configuration B

The IV line can also be re-directed by looping the tube through the device as shown in the image.

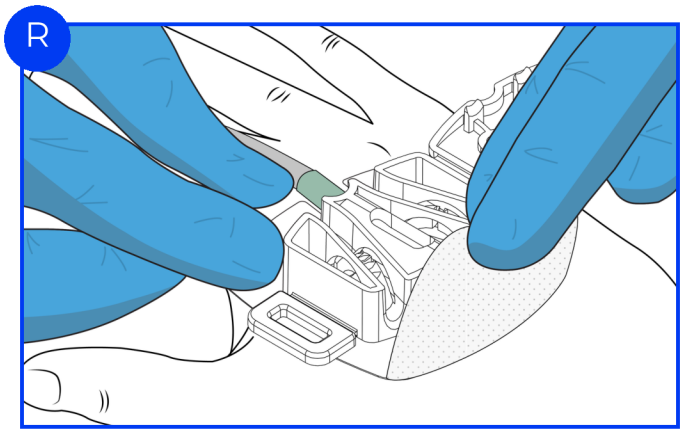

Device Removal To remove, open the cover, gently remove tubing from the channel. While holding the catheter in place, peel the protective dressing off the skin. The catheter, protective dressing and SureSet device may then be removed in one motion. Dispose of device according to hospital protocol.