
HLB-B1a · F · age not recorded · position B1 · tether arm A

neurosurveillance-eeg · HLB-fem-profsurgery-troubleshooting

allego_2__uid0802-01-46-57

post-surgery day not recorded · day 3 post-tether · body weight not recorded · duration unknown · ZT span unknown · criterion HUM · QC epoch 10 s

LIFE TIMELINE

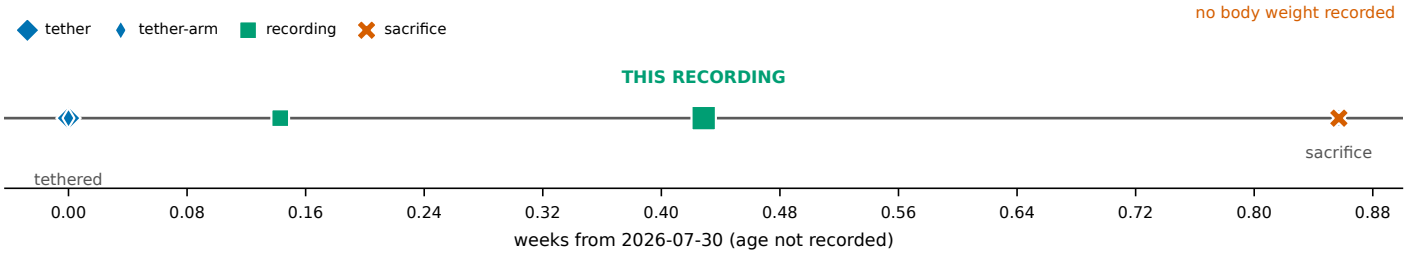

VERDICT LADDER

✓ 0 FILE — PASS

Is the recording file physically sound?

78,267,520 samples, 21.74 h

vs data samples == timestamp samples, remainder 0

78,267,520 data samples = 78,267,520 timestamp samples, remainder 0 and 0

✓ 1 IDENTITY — PASS

Which native channels belong to this animal?

EEG B/1 EMG B/2

vs layout derived from the file, never assumed

2 channels resolved from sensors_by_port; 112 wire-free inputs available as an in-file floor

✗ 2 CONNECTION — FAIL

Is the electrode connected, judged against wire-free inputs in the same file?

0.0% usable, longest unbroken block 0.0 min

vs 60 Hz < 139.6 uV (p1 of 112 wire-free inputs in this file), rms 10-150 uV, zero railed samples

no epoch passes on every role; weakest is EMG at 0.0%

– 3 SCOREABILITY — BLOCKED

Can the sleep question even be asked?

rung 2 CONNECTION did not pass

– 4 ARCHITECTURE — BLOCKED

What did the animal do?

rung 3 SCOREABILITY did not pass


– 5 EXPORT — BLOCKED

Can a human check us?

rung 3 SCOREABILITY did not pass

A rung is not evaluated if the rung below it failed: it reads BLOCKED. ? INSUFFICIENT means the question could not be asked, which is NOT the same as ✗ FAIL.

RUNG 2 evidence — usable epochs against the in-file wire-free floor

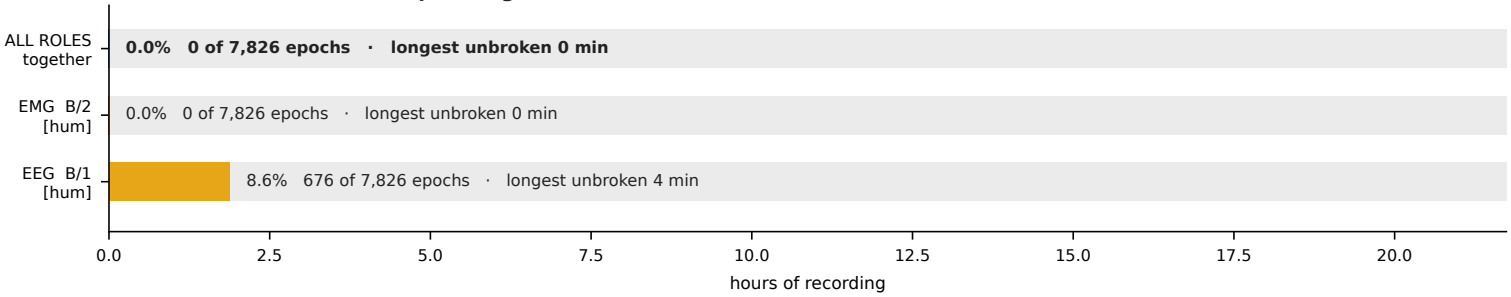

falsification: the same criterion scores the 112 wire-free inputs in this file at 0.88% usable, and must be near zero · floor 60 Hz p1 140 uV, 1-40 Hz slope p1 -3.33

– RUNG 4 ARCHITECTURE: BLOCKED

rung 3 SCOREABILITY did not pass

NO PANEL IS DRAWN FOR A RUNG THAT DID NOT PASS.

THE ORIGINAL B1. Sacrificed on 2026-08-05 because its skull electrode physically detached: the only direct physical evidence of an implant-level problem anywhere in this cohort. Carried arm A, then arm B on its last day, where its EEG went from 5 flips and a median of 2.913 MOhm to zero flips and a median of 0.903 MOhm. Arm C was never run on it. ⚠An earlier vault write-up recorded this as an anaesthesia death, and the welfare action taken from that, were both withdrawn on 2026-08-09.

HLB-fem-profsurgery-troubleshooting · card schema v2 · generated 2026-08-09T11:12:04+09:00 · git not a git repo · thresholds c635d5245a5b (qc_thresholds.py) · criterion HUM at 10 s epochs. SLOPE and HUM usable fractions are NOT comparable, and neither is comparable to a fraction computed at the 4 s staging epoch.