
Figure 1. Electrode impedance of all eight rig positions, five single sweeps, 31 July to 4 August 2026

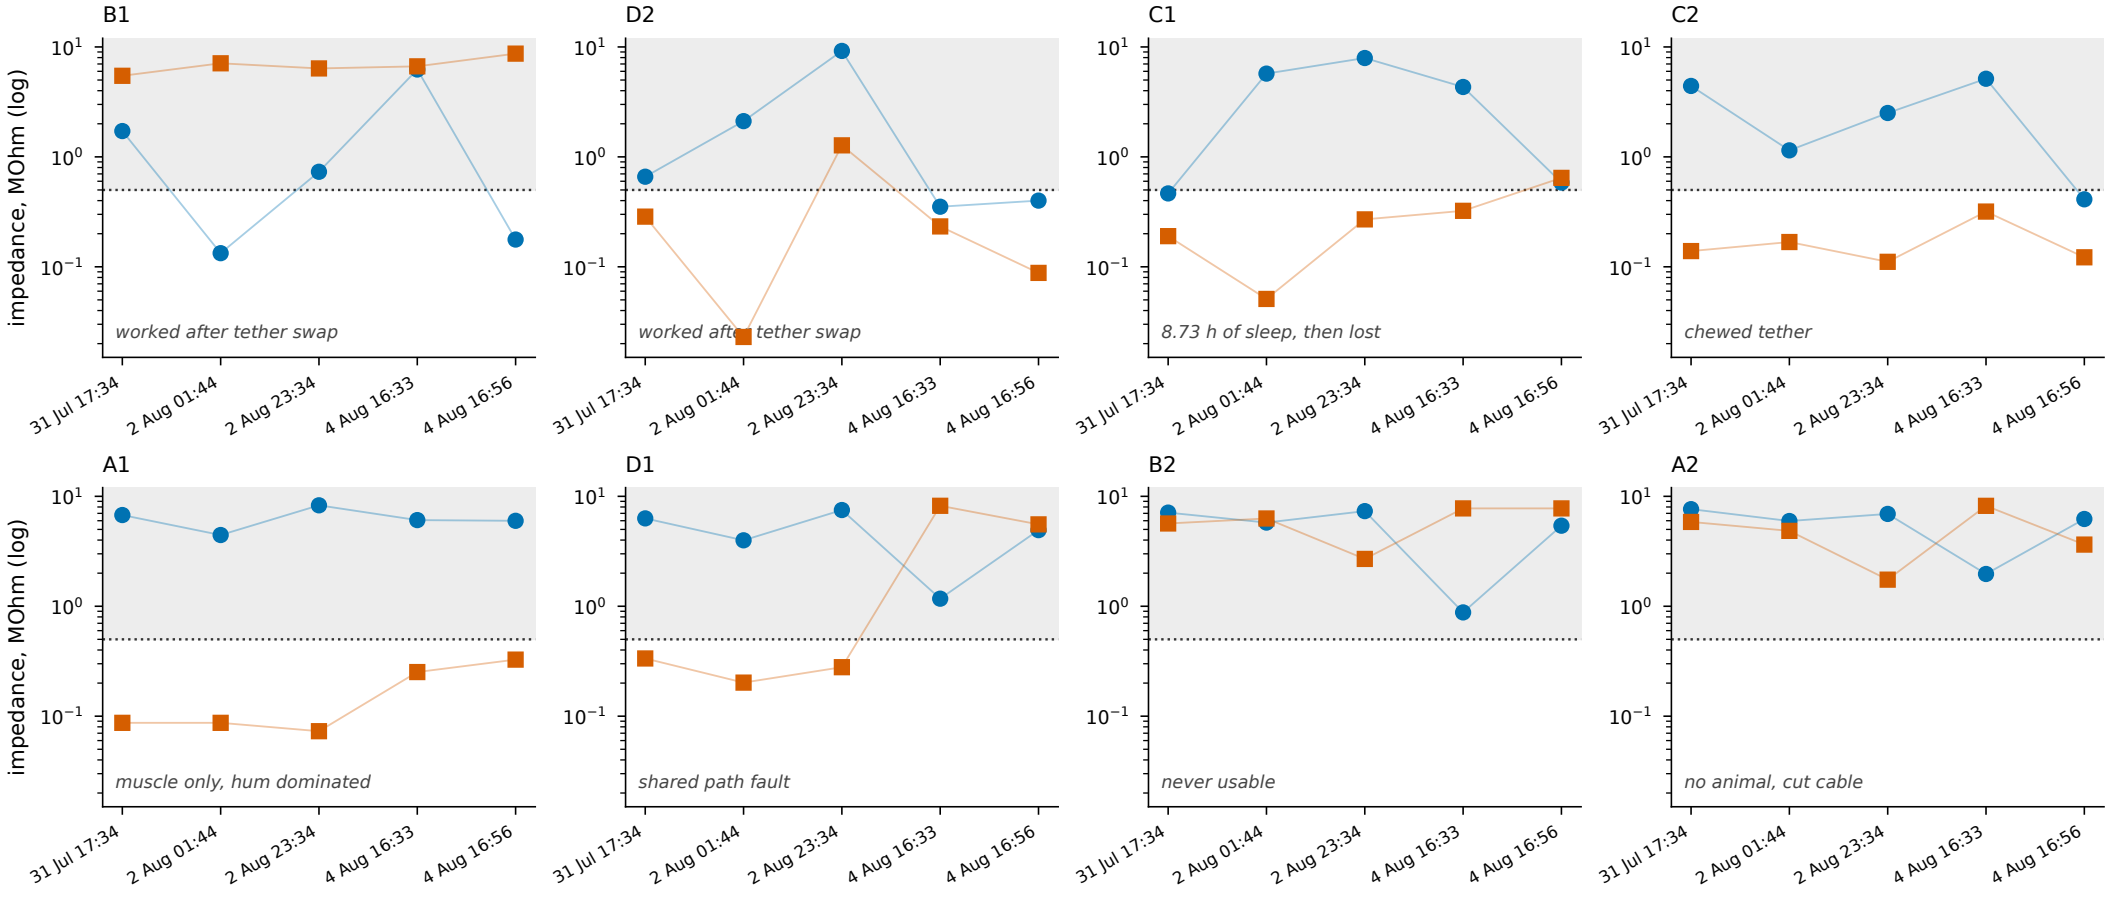

Each marker is ONE 20 second sweep, unrepeated, so no marker carries an interval and the faint connector indicates reading order only, not a measured trajectory. Nothing was done to any animal between sweeps. Shaded region above the dotted line is the range in which a reading cannot be told apart from an amplifier input with no wire attached. Measurement: Intan RHD2216 on chip impedance check at 1 kHz, magnitude only, positive input of each bipolar pair. Every position moves in both directions and none declines monotonically, which is not the pattern of a failing implant.