

Figure 8. Statistics behind the hardware claims

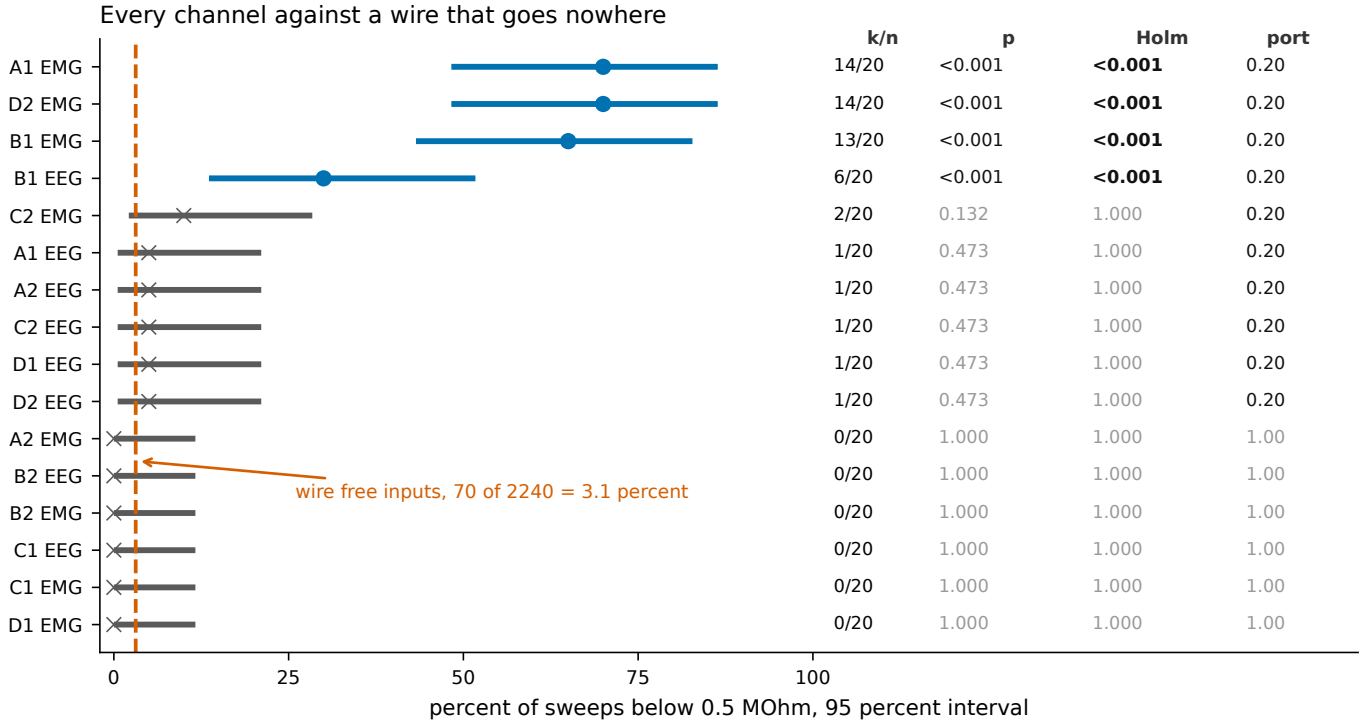

	k/n	p	Holm	port
A1 EMG	14/20	<0.001	**<0.001**	0.20
D2 EMG	14/20	<0.001	**<0.001**	0.20
B1 EMG	13/20	<0.001	**<0.001**	0.20
B1 EEG	6/20	<0.001	**<0.001**	0.20
C2 EMG	2/20	0.132	1.000	0.20
A1 EEG	1/20	0.473	1.000	0.20
A2 EEG	1/20	0.473	1.000	0.20
C2 EEG	1/20	0.473	1.000	0.20
D1 EEG	1/20	0.473	1.000	0.20
D2 EEG	1/20	0.473	1.000	0.20
A2 EMG	0/20	1.000	1.000	1.00
B2 EEG	0/20	1.000	1.000	1.00
B2 EMG	0/20	1.000	1.000	1.00
C1 EEG	0/20	1.000	1.000	1.00
C1 EMG	0/20	1.000	1.000	1.00
D1 EMG	0/20	1.000	1.000	1.00

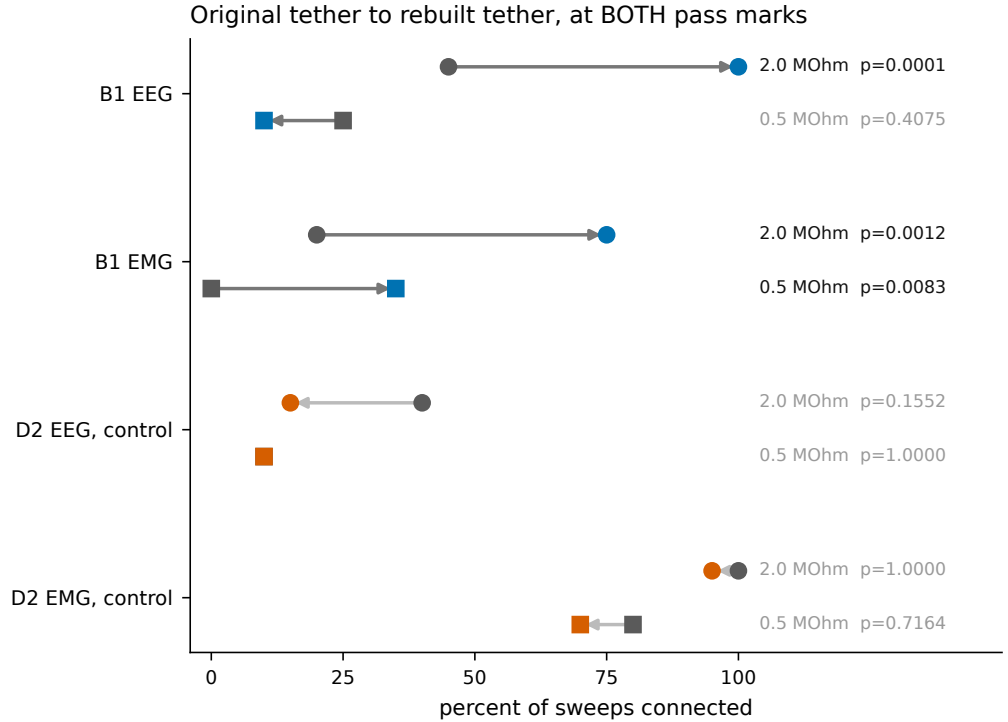

LEFT. Each channel measured 20 times over 11 minutes on 6 August, against every amplifier input on the same chips with no wire attached, read in the same sweeps: 2240 readings. Fisher exact, one sided, with Jeffreys 95 percent intervals. Holm adjusts for the 16 tests against one shared comparison group; only 4 channels survive it, and three of those are muscle channels, so exactly ONE animal had a usable EEG that day. The final column is a cluster aware check: the observed rate compared against the four PORT level floor rates, since 2,240 readings from 4 ports are not 2,240 independent draws. It has no power at four clusters and is shown so the reader can see that, not as a second opinion. RIGHT. The tether comparison of 5 August at both pass marks. At 2 MOhm, the threshold in use that day, B1's EEG goes 9 of 20 to 20 of 20. At the corrected 0.5 MOhm pass mark, adopted the next day once a cut cable was found to pass 22 percent of the time at 2 MOhm, the SAME BLOCKS give 5 of 20 to 2 of 20: the EEG improvement disappears and reverses, while the muscle channel still improves. The tether conclusion therefore rests on the RECORDING, where D2 went from 0.0 to 87.9 percent usable, not on this impedance block.