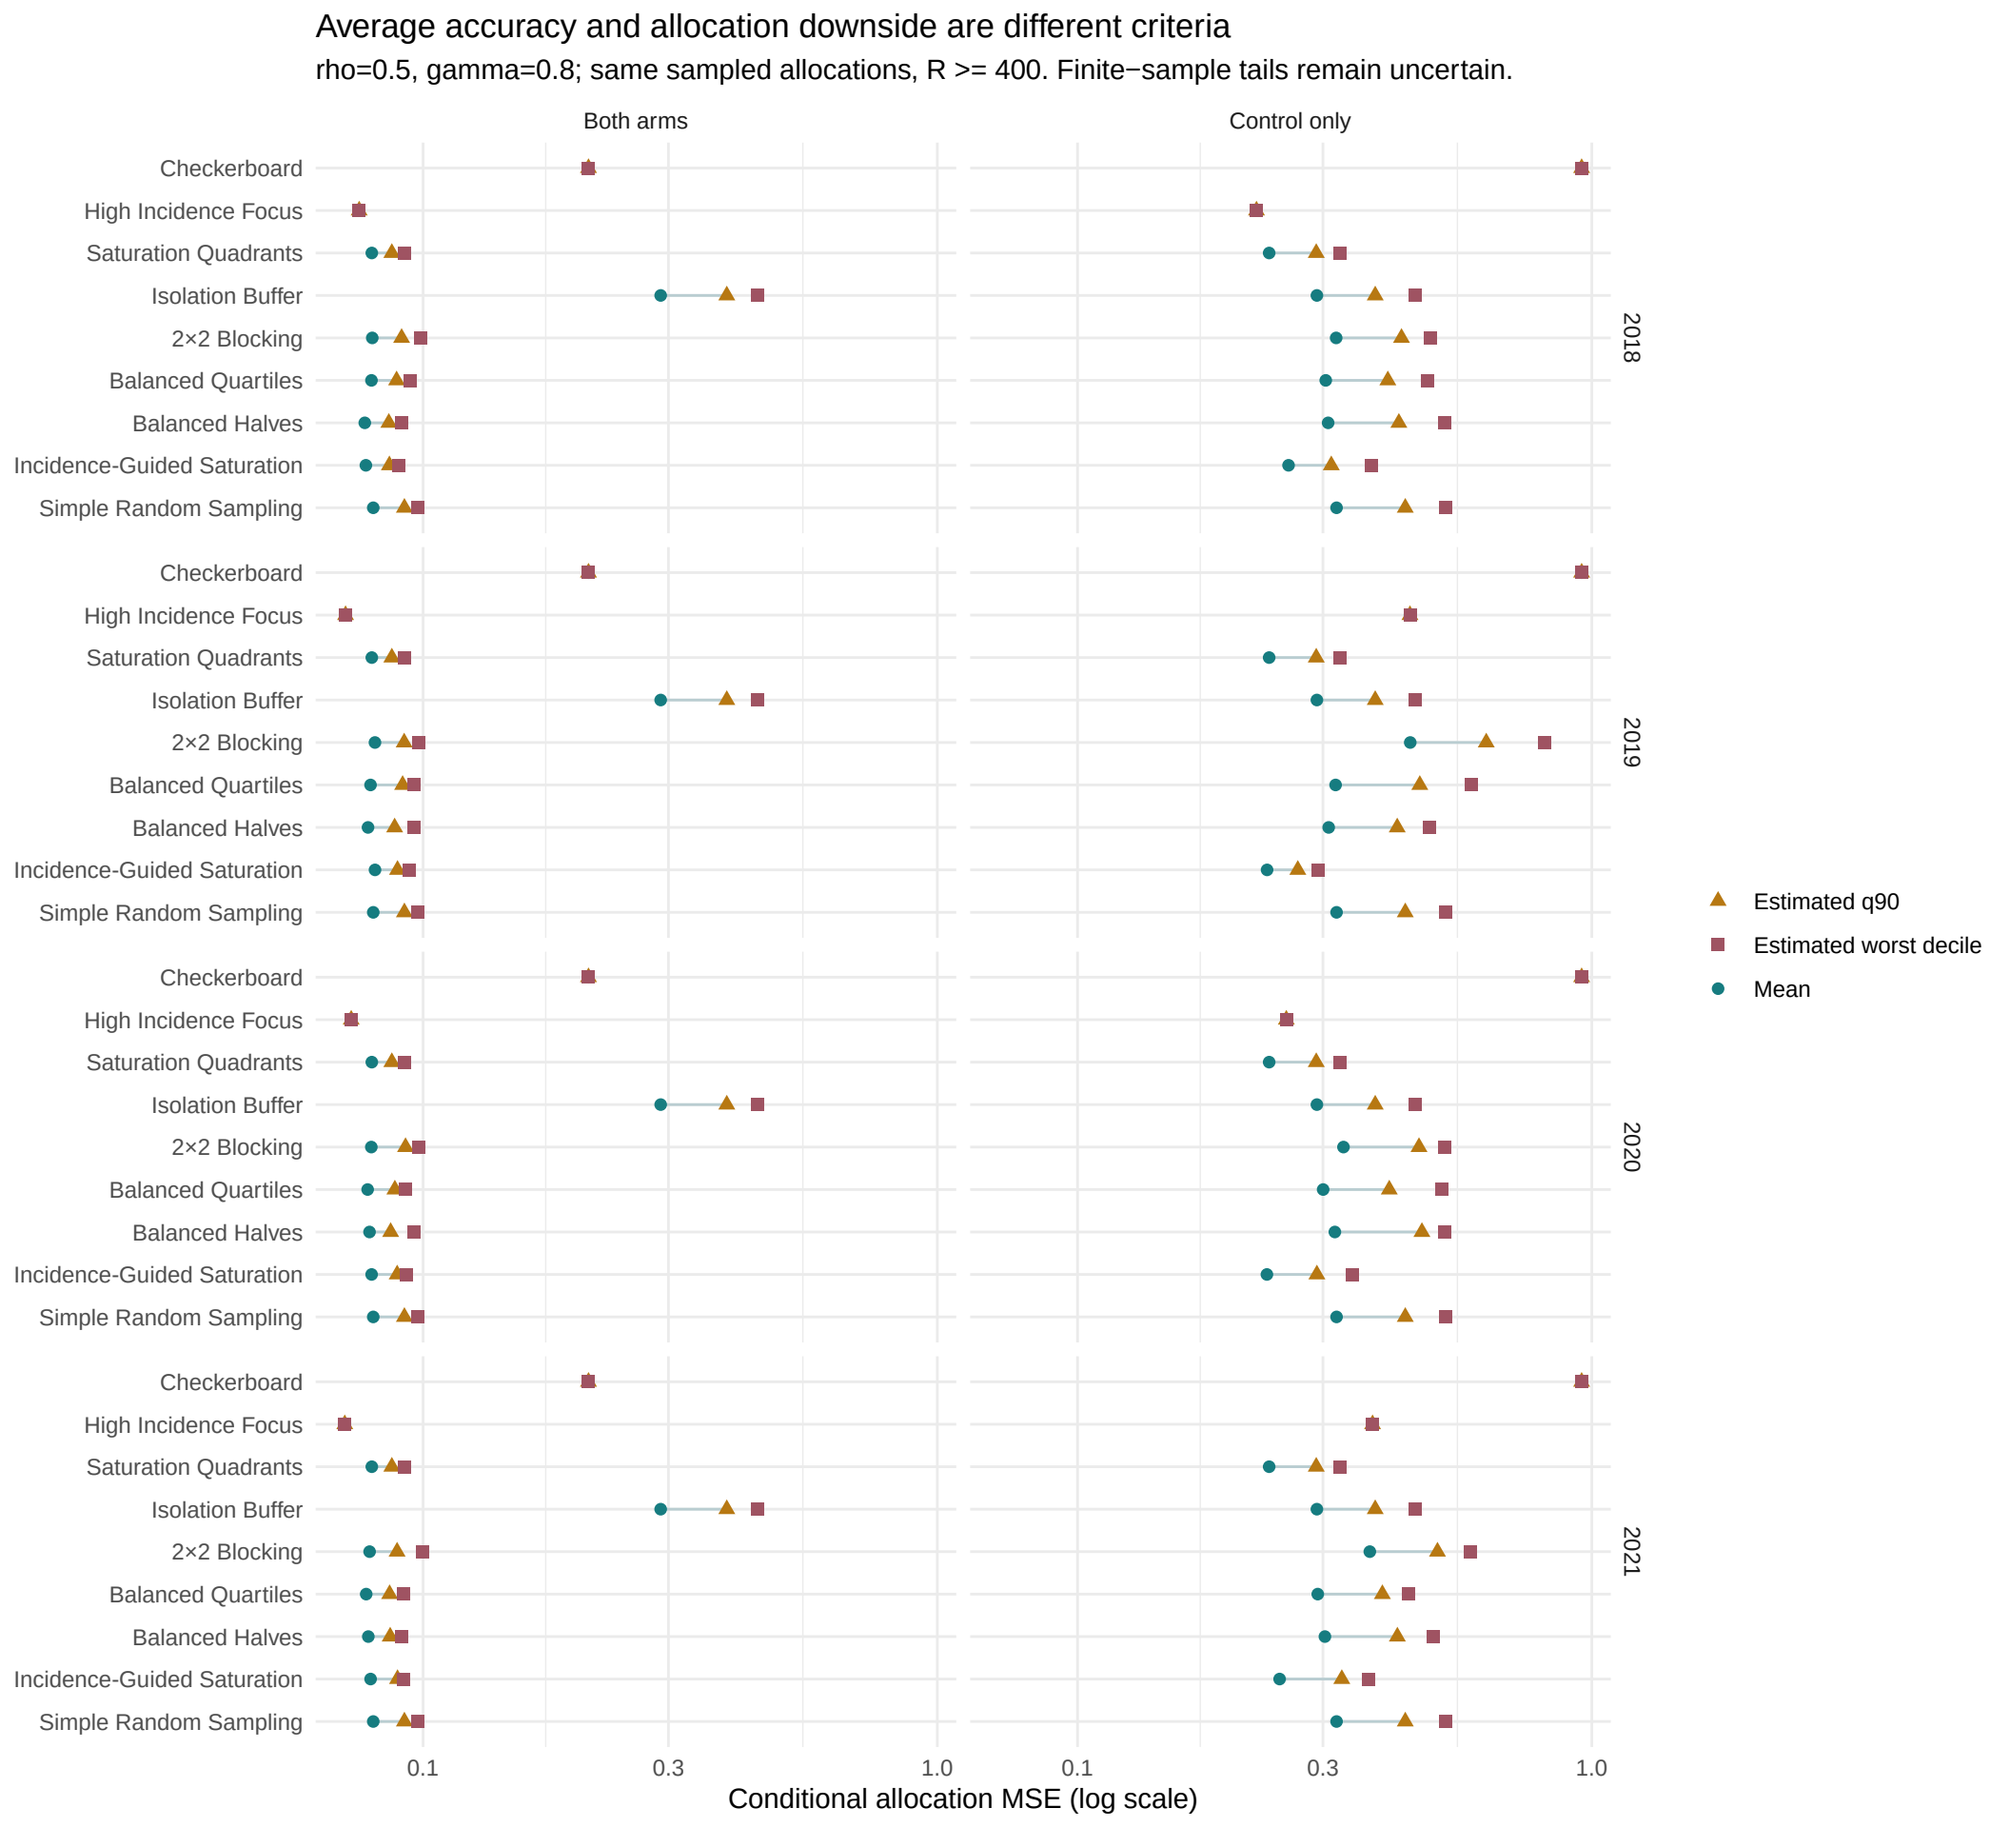
Average accuracy and allocation downside are different criteria
rho=0.5, gamma=0.8; same sampled allocations, R >= 400. Finite−sample tails remain uncertain.
Both arms
Control only
Checkerboard
High Incidence Focus
Saturation Quadrants
Isolation Buffer
2×2 Blocking
Balanced Quartiles
Balanced Halves
Incidence-Guided Saturation
Simple Random Sampling
2018
2019
2020
2021
Estimated q90
Estimated worst decile
Mean
0.1
0.3
1.0
Conditional allocation MSE (log scale)