

AO/PI

Sample Name:	Sample Name	Created Date/Time:	2024-11-15 10:34:58
Account:	General	Passage:	
Software Version:	v4.1.0	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20241115103458
Description:			

Results

Last Processed Date/Time:	2024-11-15 10:34:58	Gating Min Diameter (um):	4
Gating Max Diameter (um):	30	Live Cell Count:	110
Dead Cell Count:	117	Total Cell Count:	227
% Viability:	48.4581	Mean Diameter (um):	11.16
Live Cells/mL:	6.47e+05	Dead Cells/mL:	6.88e+05
Total Cells/mL:	1.33e+06		


Dilution

Target Cells/mL:	5.00e+03	Target Number of Cells:	N/A
Target Volume (mL):	5	Original Volume (mL):	10
Dilution Guidance:			


Protocol

Protocol:	New Protocol Name	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	4	Protocol Max Diameter (um):	30
Live Roundness:	20	Dead Roundness:	10
Green Fluorescence Threshold:	10	Red Fluorescence Threshold:	1
Irregular Cell Mode:	False		

Sample Images

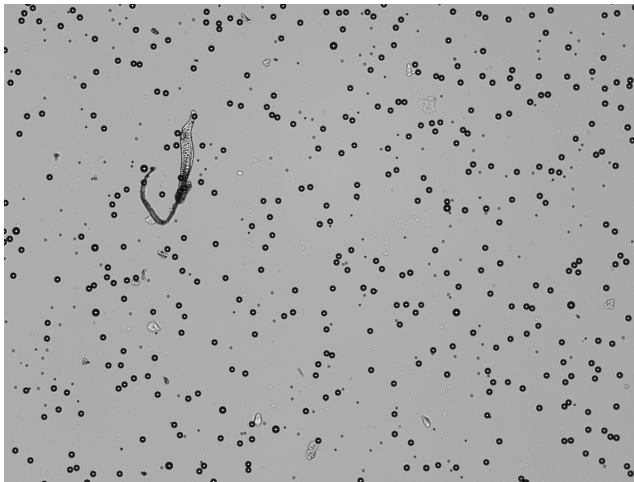


Brightfield

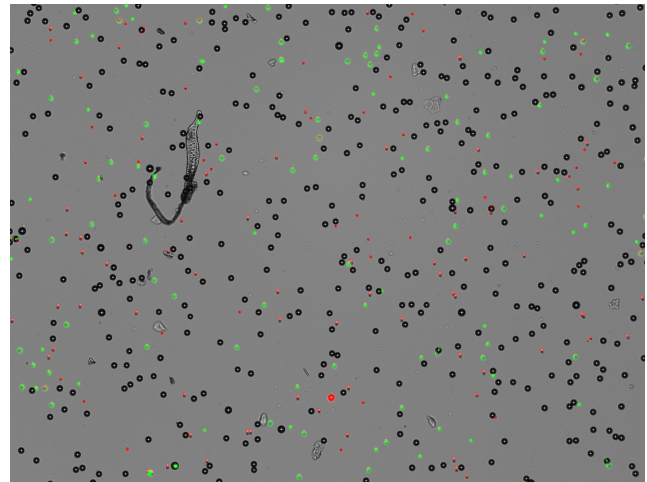


Counted


Sample Histograms

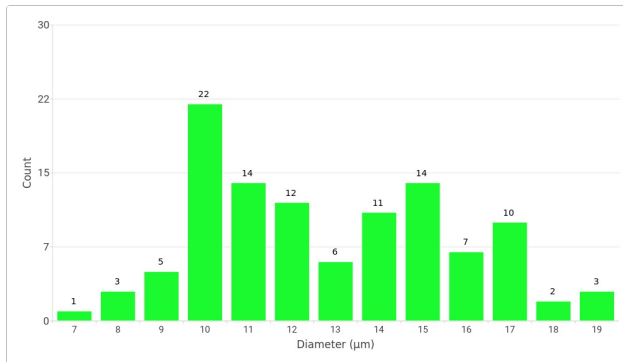


Live Cells (by Size)

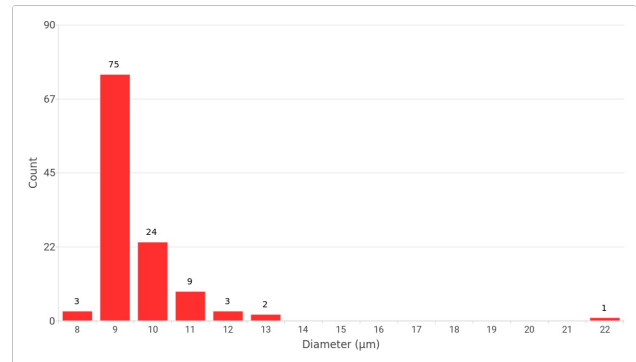


Dead Cells (by Size)

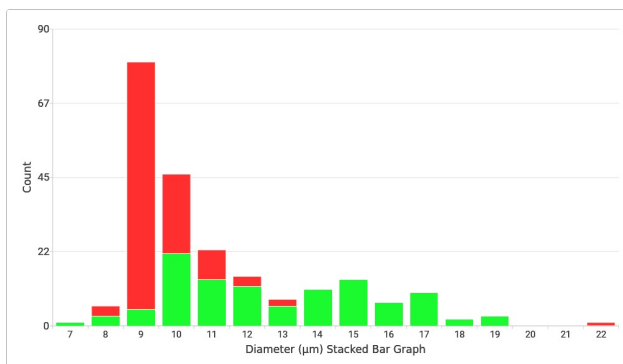

Live+Dead Cells (by Size)

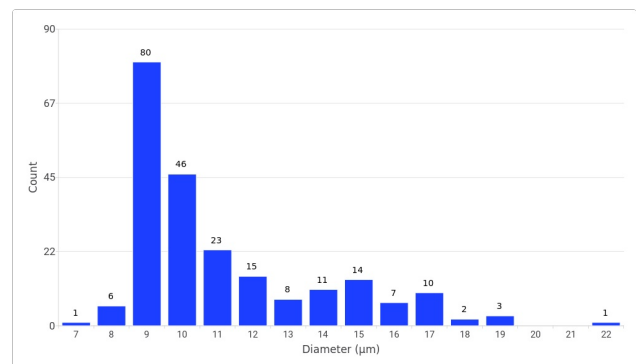

Total Cells (by Size)

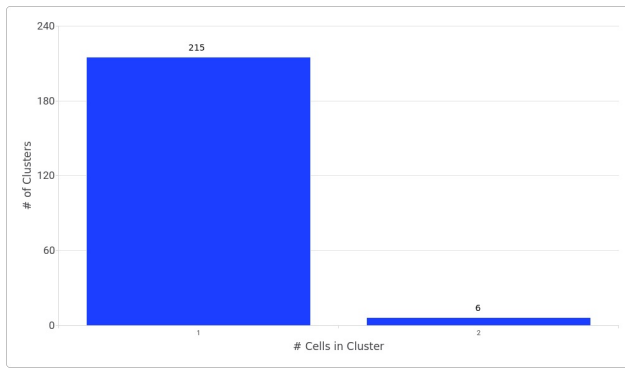

Cluster Size