

AO/PI

Sample Name:	Sample Name	Created Date/Time:	2025-03-27 09:35:52
Account:	General	Passage:	
Software Version:	v4.1.8	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20250327093552
Description:			

Results

Last Processed Date/Time:	2025-03-27 09:35:52	Gating Min Diameter (um):	4
Gating Max Diameter (um):	30	Live Cell Count:	45
Dead Cell Count:	44	Total Cell Count:	89
% Viability:	50.5618	Mean Diameter (um):	11.75
Live Cells/mL:	2.65e+05	Dead Cells/mL:	2.59e+05
Total Cells/mL:	5.23e+05		


Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			


Protocol

Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	4	Protocol Max Diameter (um):	30
Live Roundness:	1	Dead Roundness:	1
Green Fluorescence Threshold:	1	Red Fluorescence Threshold:	1
Irregular Cell Mode:	False		

Sample Images

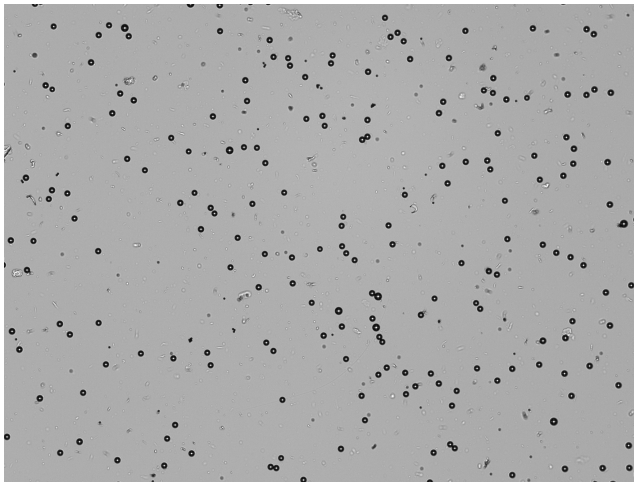


Brightfield

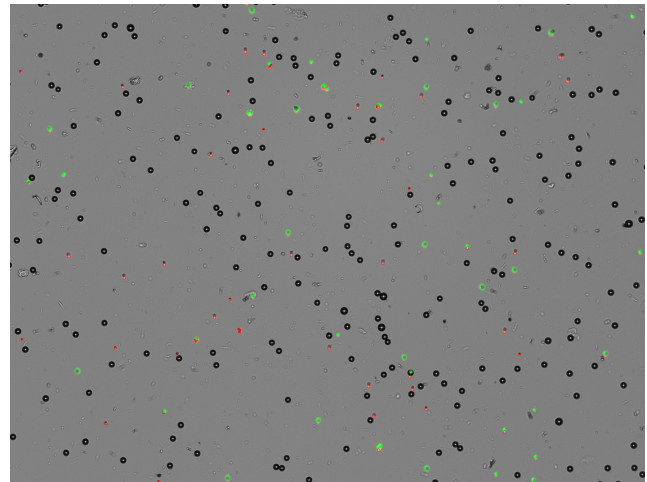


Counted


Sample Histograms

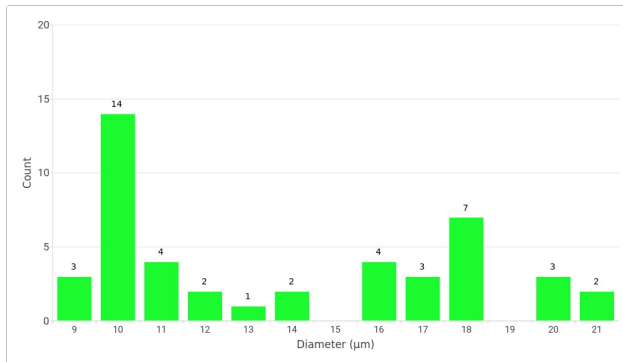


Live Cells (by Size)

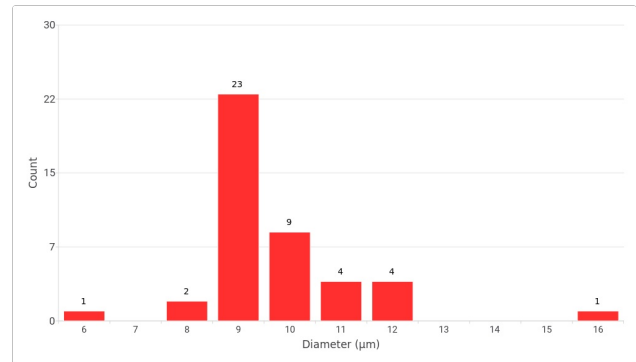


Dead Cells (by Size)

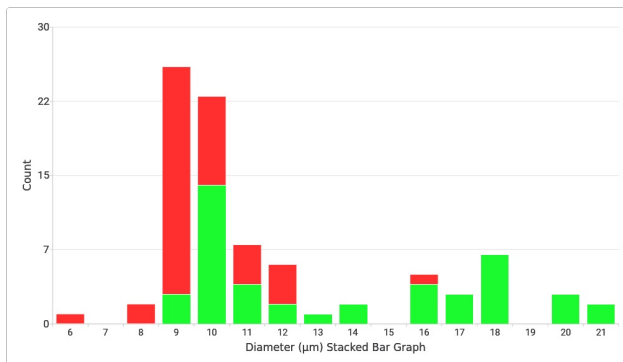

Live+Dead Cells (by Size)

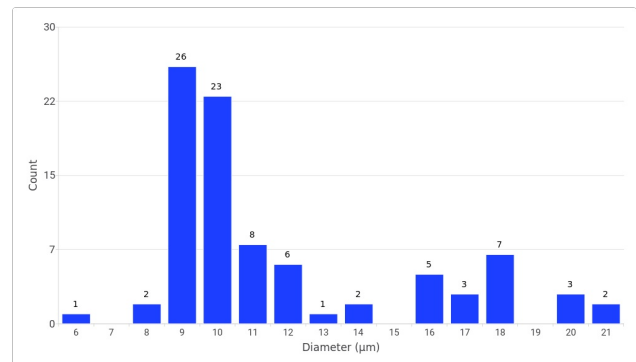

Total Cells (by Size)

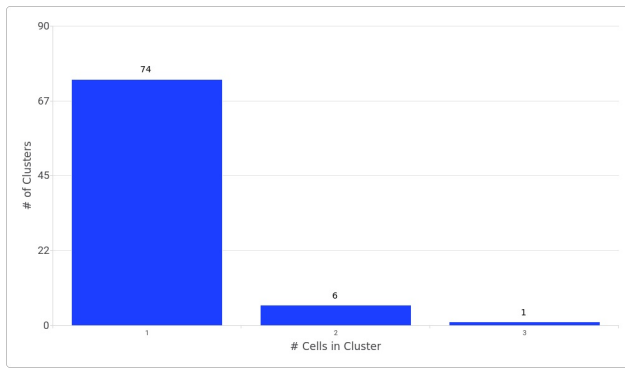

Cluster Size