

AO/PI

Sample Name:	Sample Name	Created Date/Time:	2025-03-27 09:38:07
Account:	General	Passage:	
Software Version:	v4.1.8	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20250327093807
Description:			

Results

Last Processed Date/Time:	2025-03-27 09:38:07	Gating Min Diameter (um):	4
Gating Max Diameter (um):	30	Live Cell Count:	20
Dead Cell Count:	31	Total Cell Count:	51
% Viability:	39.2157	Mean Diameter (um):	10.94
Live Cells/mL:	1.18e+05	Dead Cells/mL:	1.82e+05
Total Cells/mL:	3.00e+05		


Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			


Protocol

Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	4	Protocol Max Diameter (um):	30
Live Roundness:	1	Dead Roundness:	1
Green Fluorescence Threshold:	1	Red Fluorescence Threshold:	1
Irregular Cell Mode:	False		

Sample Images




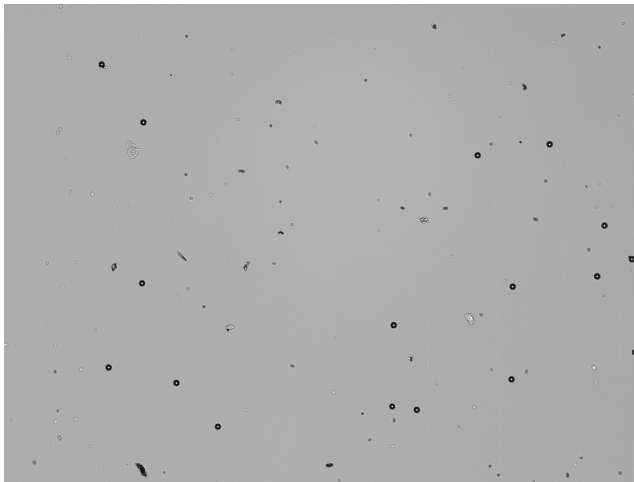



Brightfield

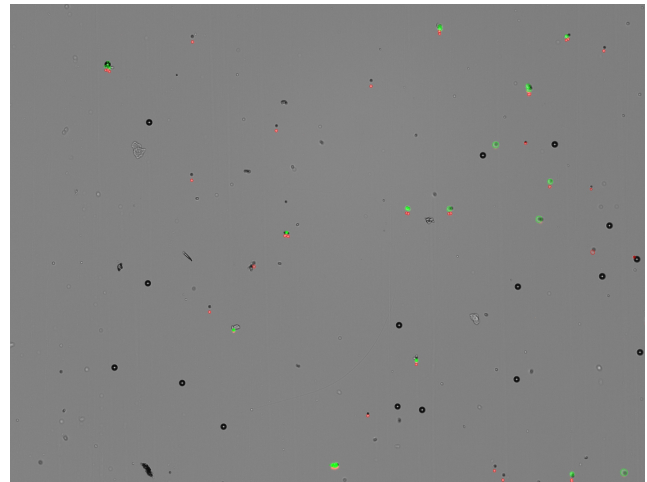

Counted

Sample Histograms

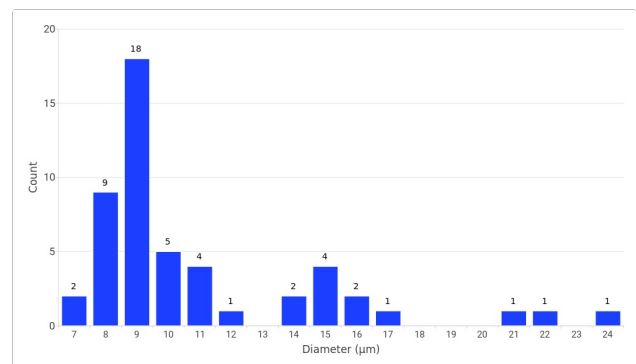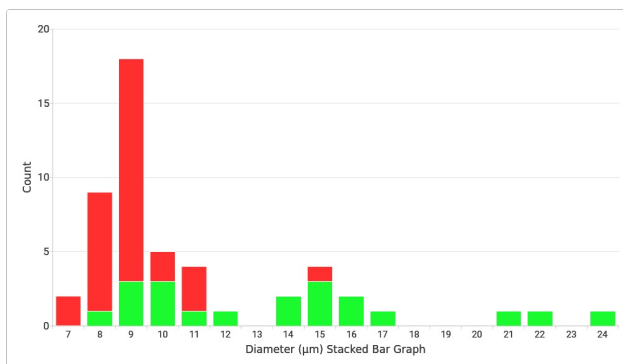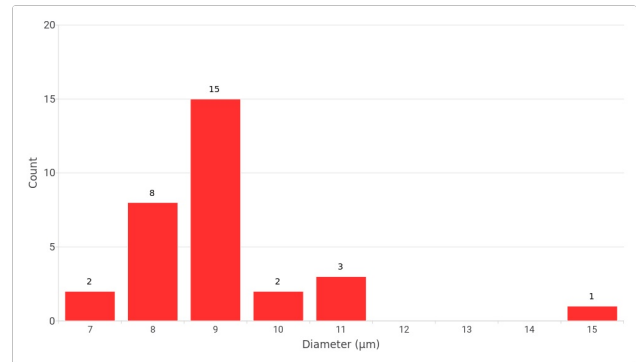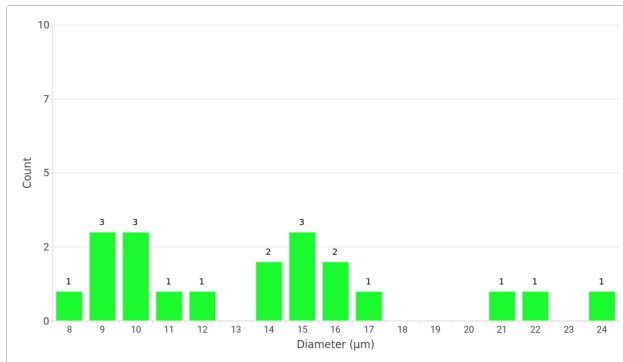

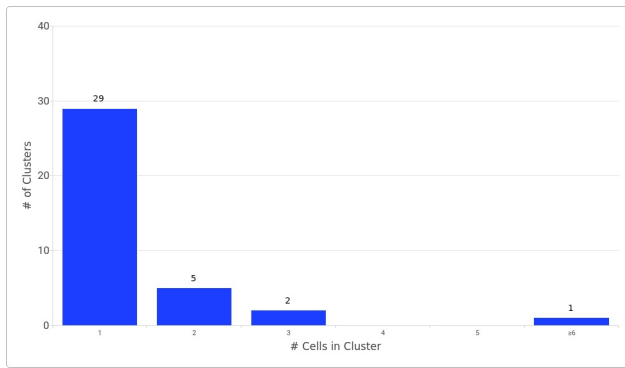

Cluster Size