

Trypan Blue Tissue Culture

Sample Name:	Sample Name	Created Date/Time:	2025-03-27 11:47:32
Account:	General	Passage:	
Software Version:	v4.1.8	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20250327114732
Description:			

Results

Last Processed Date/Time:	2025-03-27 11:47:32	Gating Min Diameter (um):	10
Gating Max Diameter (um):	18	Live Cell Count:	517
Dead Cell Count:	134	Total Cell Count:	651
% Viability:	79.4163	Mean Diameter (um):	14.49
Live Cells/mL:	3.04e+06	Dead Cells/mL:	7.88e+05
Total Cells/mL:	3.83e+06		



Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			





Protocol


Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	10	Protocol Max Diameter (um):	18
Live Roundness:	50	Dead Roundness:	25
Stained Threshold:	35		
Small Cell Mode:	False		
Irregular Cell Mode:	False		

Sample Images

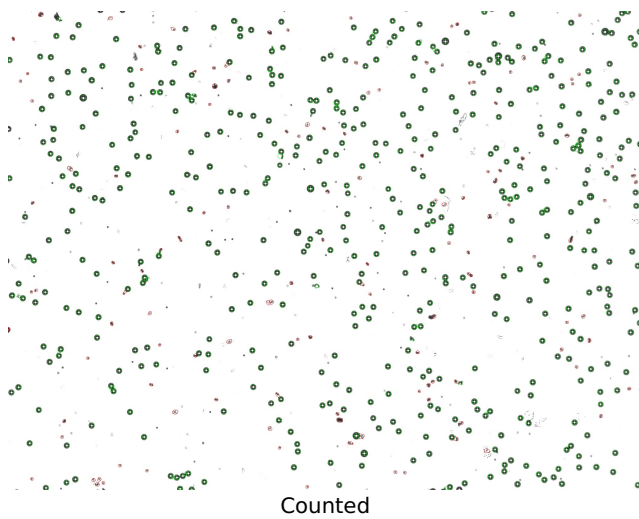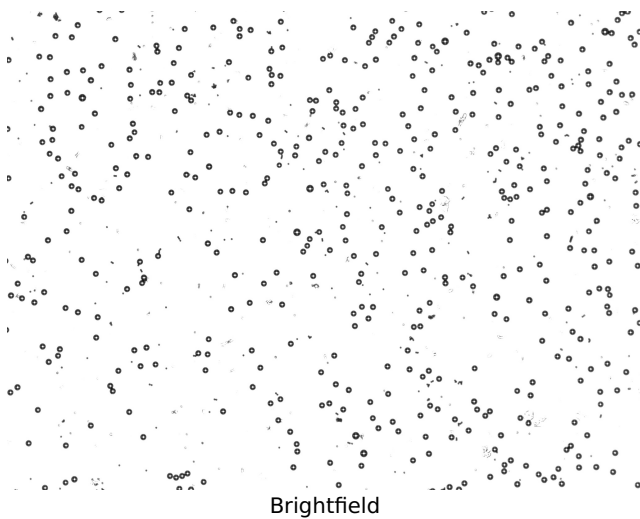

Sample Histograms

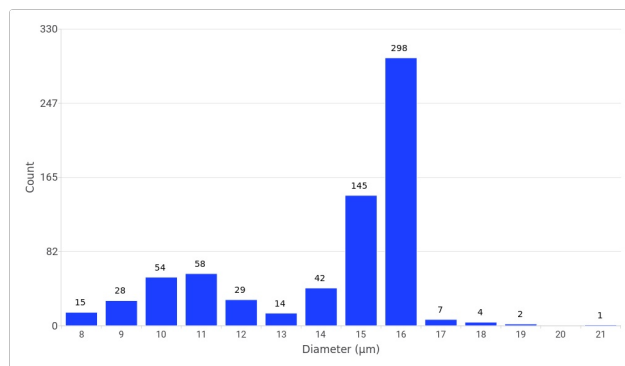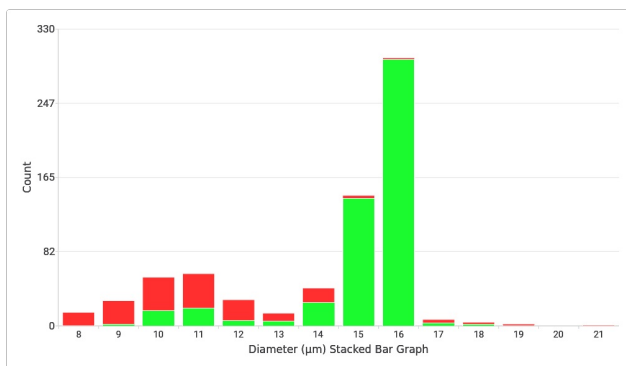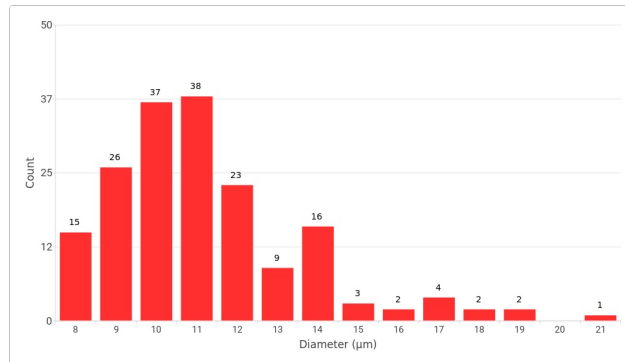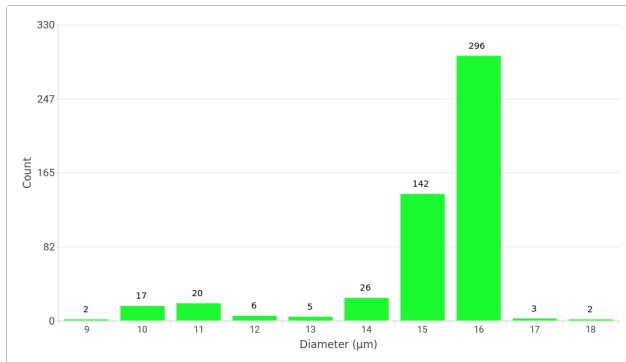

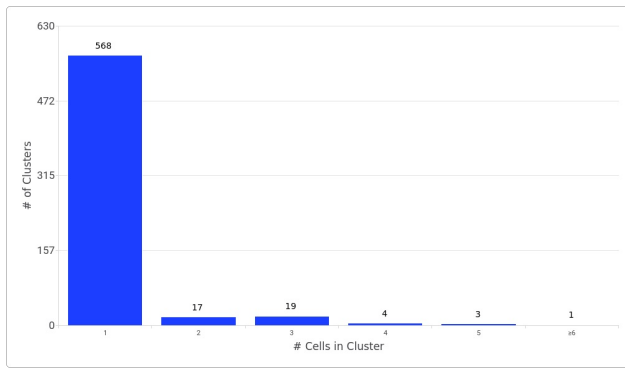

Cluster Size