

Trypan Blue Tissue Culture

Sample Name:	Sample Name	Created Date/Time:	2025-04-04 10:40:53
Account:	General	Passage:	
Software Version:	v4.1.8	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20250404104053
Description:			

Results

Last Processed Date/Time:	2025-04-04 10:40:53	Gating Min Diameter (um):	6
Gating Max Diameter (um):	30	Live Cell Count:	85
Dead Cell Count:	215	Total Cell Count:	300
% Viability:	28.3333	Mean Diameter (um):	13.25
Live Cells/mL:	5.00e+05	Dead Cells/mL:	1.26e+06
Total Cells/mL:	1.76e+06		



Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			





Protocol


Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	6	Protocol Max Diameter (um):	30
Live Roundness:	50	Dead Roundness:	25
Stained Threshold:	35		
Small Cell Mode:	False		
Irregular Cell Mode:	False		

Sample Images

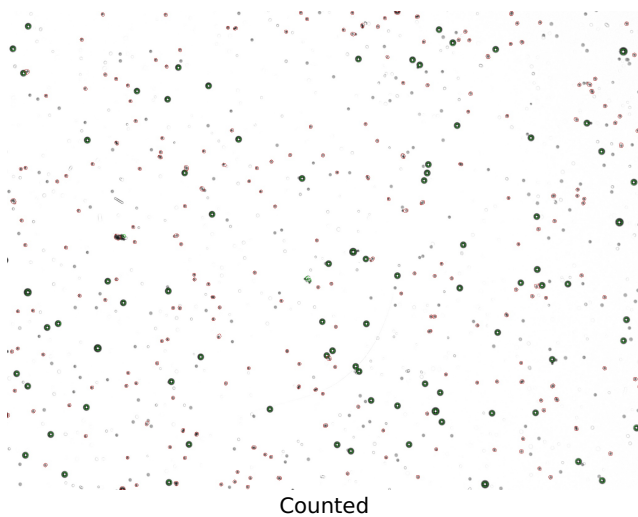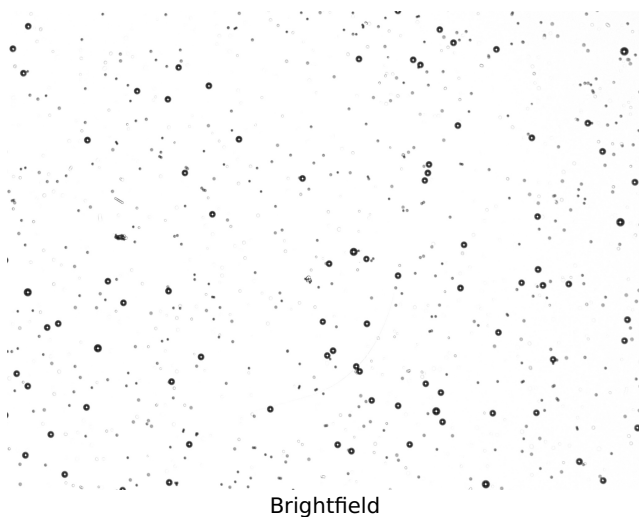

Sample Histograms

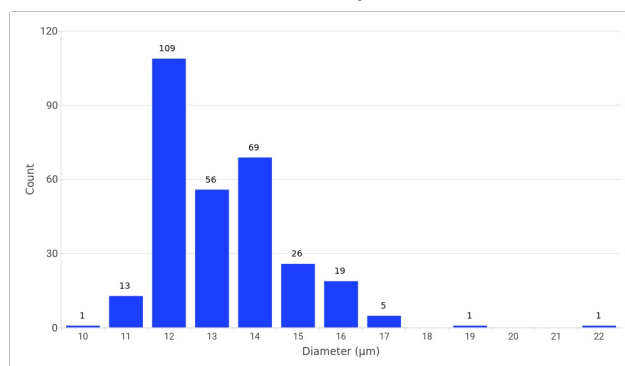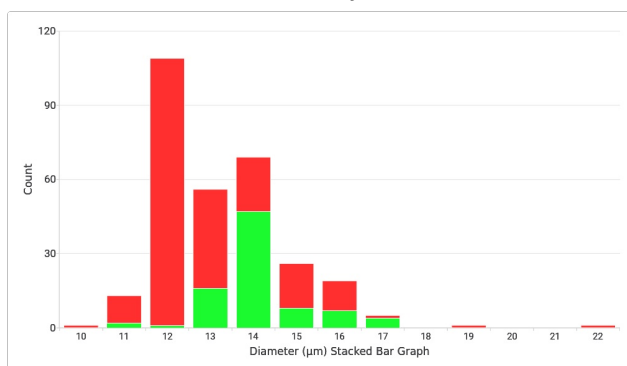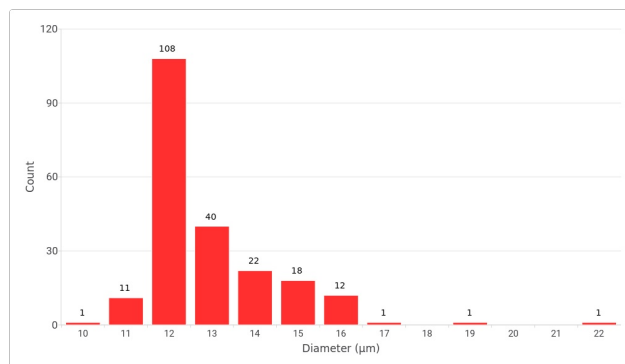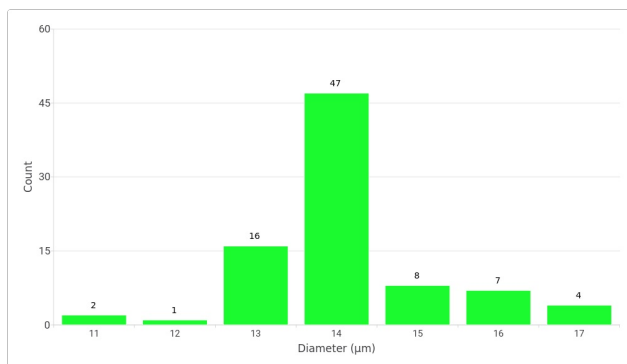

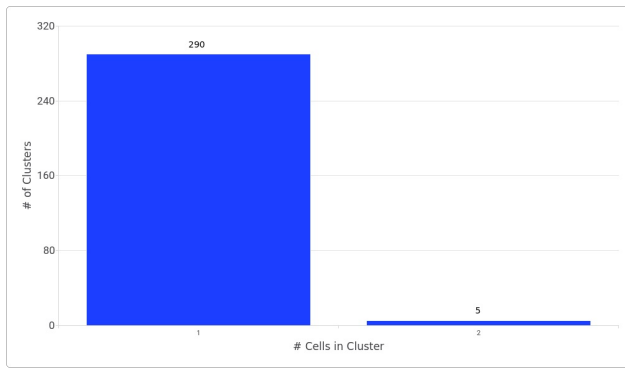

Cluster Size