

Trypan Blue Tissue Culture

Sample Name:	Sample Name	Created Date/Time:	2025-04-04 10:47:19
Account:	General	Passage:	
Software Version:	v4.1.8	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20250404104719
Description:			

Results

Last Processed Date/Time:	2025-04-04 10:53:01	Gating Min Diameter (um):	7
Gating Max Diameter (um):	21	Live Cell Count:	29
Dead Cell Count:	361	Total Cell Count:	390
% Viability:	7.4359	Mean Diameter (um):	10.43
Live Cells/mL:	1.70e+05	Dead Cells/mL:	2.12e+06
Total Cells/mL:	2.29e+06		


Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			


Protocol

Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	7	Protocol Max Diameter (um):	21
Live Roundness:	50	Dead Roundness:	50
Stained Threshold:	65		
Small Cell Mode:	False		
Irregular Cell Mode:	False		

Sample Images

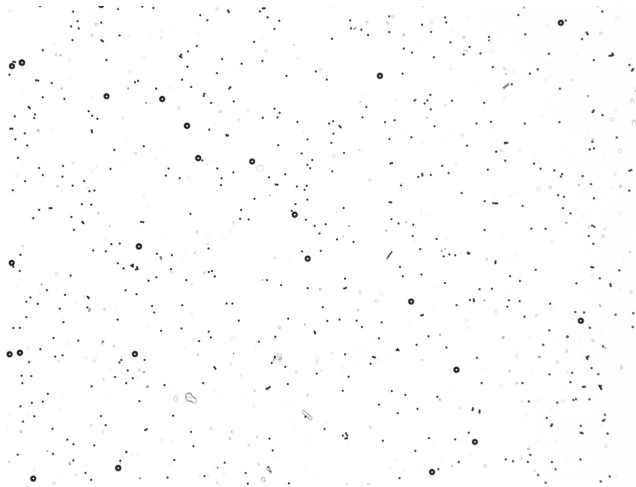


Brightfield

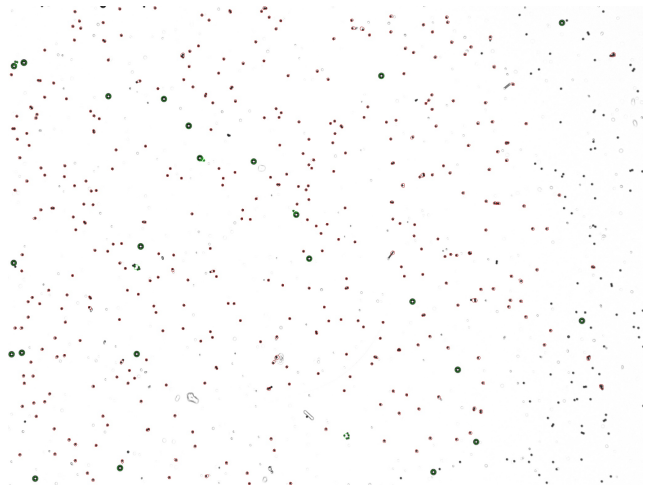


Counted


Sample Histograms

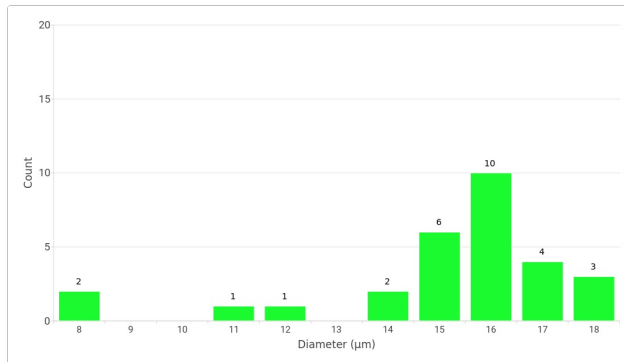


Live Cells (by Size)

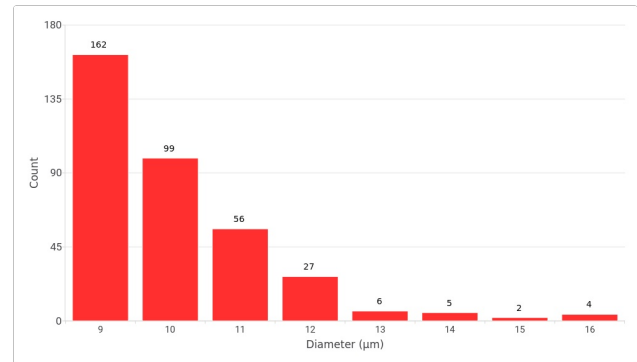


Dead Cells (by Size)

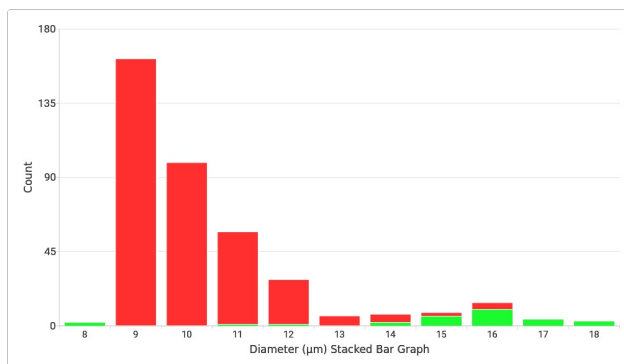

Live+Dead Cells (by Size)

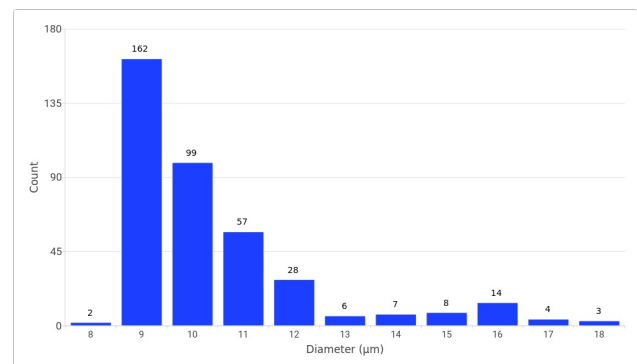

Total Cells (by Size)

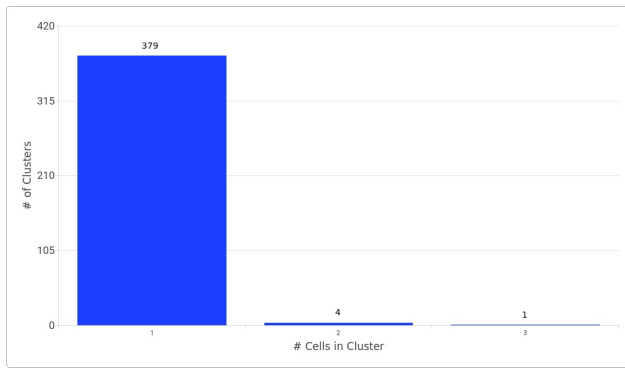

Cluster Size