

Trypan Blue Tissue Culture

Sample Name:	Sample Name	Created Date/Time:	2025-06-02 10:47:18
Account:	General	Passage:	
Software Version:	v4.1.8	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20250602104718
Description:			

Results

Last Processed Date/Time:	2025-06-02 10:47:18	Gating Min Diameter (um):	11
Gating Max Diameter (um):	16	Live Cell Count:	43
Dead Cell Count:	35	Total Cell Count:	78
% Viability:	55.1282	Mean Diameter (um):	13.69
Live Cells/mL:	2.53e+05	Dead Cells/mL:	2.06e+05
Total Cells/mL:	4.59e+05		


Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			


Protocol

Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	11	Protocol Max Diameter (um):	16
Live Roundness:	50	Dead Roundness:	25
Stained Threshold:	35		
Small Cell Mode:	False		
Irregular Cell Mode:	False		

Sample Images

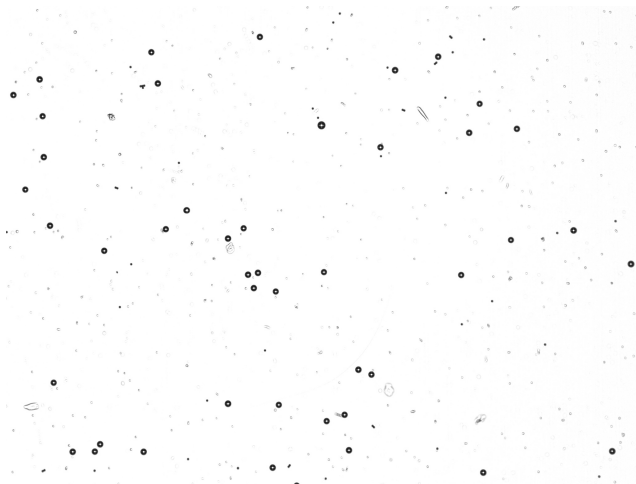


Brightfield

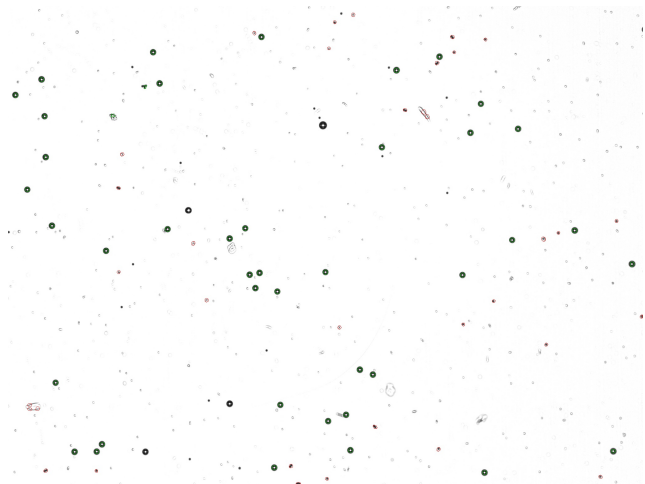


Counted


Sample Histograms

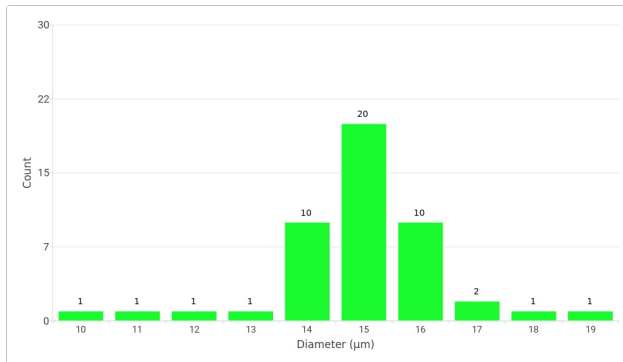


Live Cells (by Size)

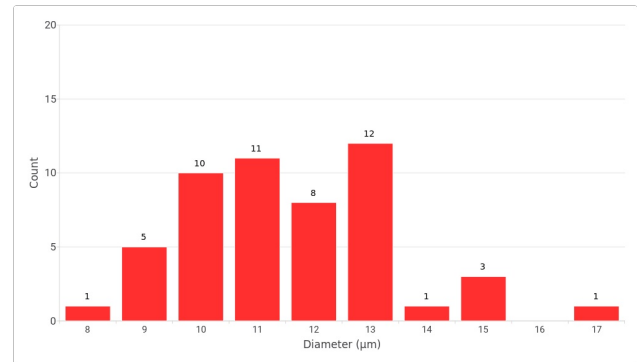


Dead Cells (by Size)

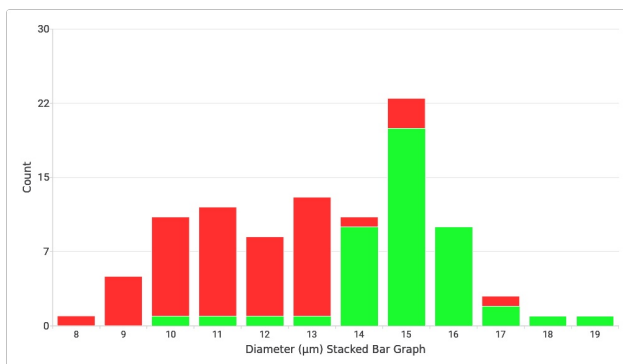

Live+Dead Cells (by Size)

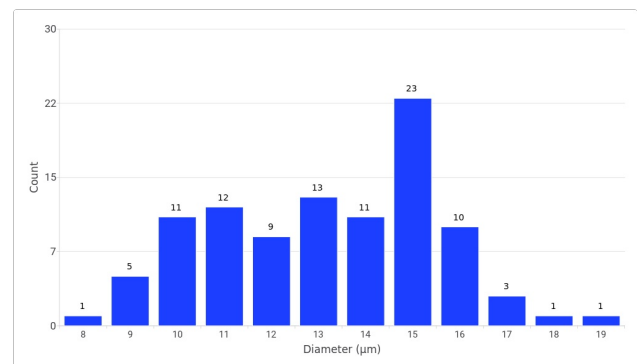

Total Cells (by Size)

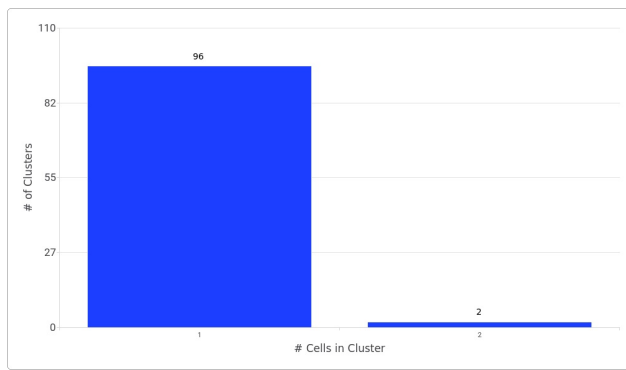

Cluster Size