

Trypan Blue Tissue Culture

Sample Name:	Sample Name	Created Date/Time:	2026-01-23 10:37:55
Account:	General	Passage:	
Software Version:	v4.3.4	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20260123103755
Description:			

Results

Last Processed Date/Time:	2026-01-23 10:37:55	Gating Min Diameter (um):	6
Gating Max Diameter (um):	20	Live Cell Count:	180
Dead Cell Count:	61	Total Cell Count:	241
% Viability:	74.6888	Mean Diameter (um):	13.56
Live Cells/mL:	1.06e+06	Dead Cells/mL:	3.59e+05
Total Cells/mL:	1.42e+06		



Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			


Protocol

Protocol:	Ssm	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	6	Protocol Max Diameter (um):	20
Live Roundness:	35	Dead Roundness:	15
Stained Threshold:	5		
Small Cell Mode:	True		
Irregular Cell Mode:	False		


Sample Images

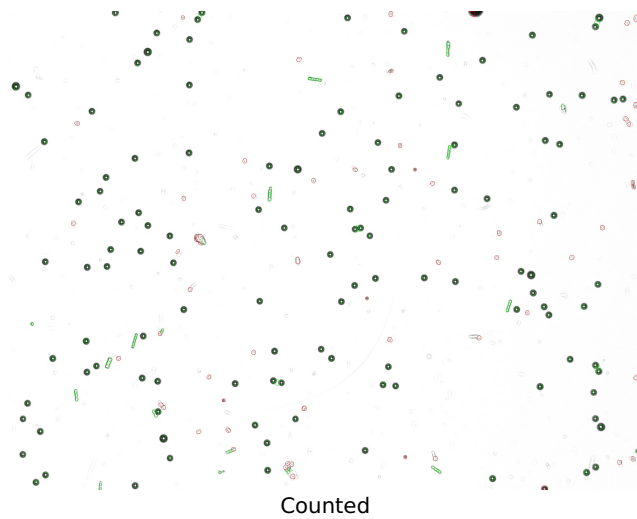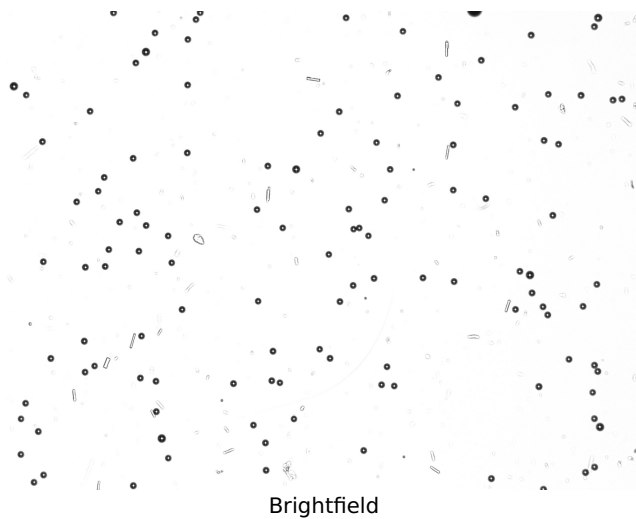


Sample Histograms

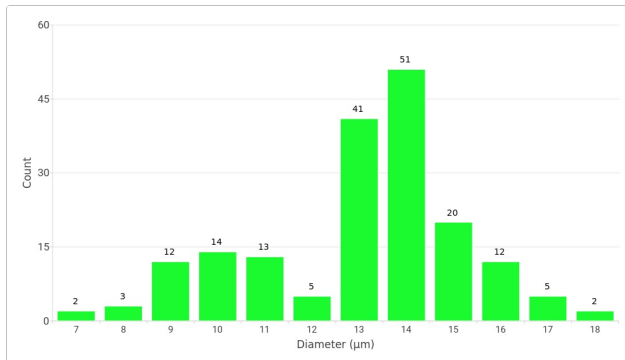


Live Cells (by Size)

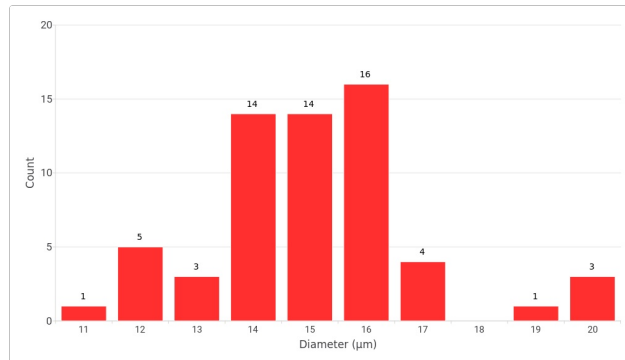


Dead Cells (by Size)

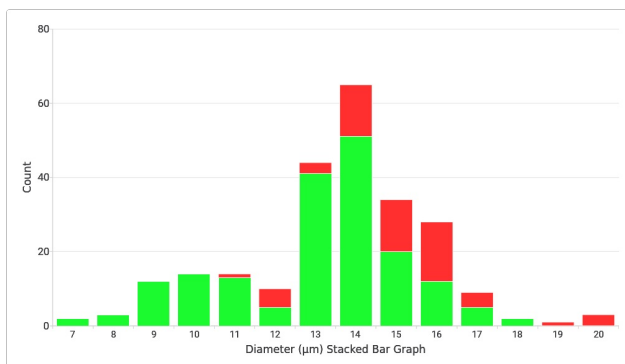

Live+Dead Cells (by Size)

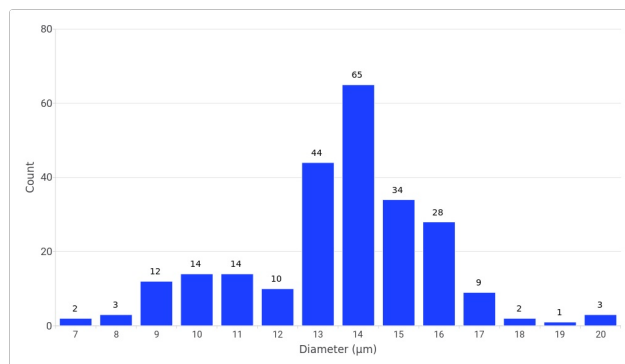

Total Cells (by Size)

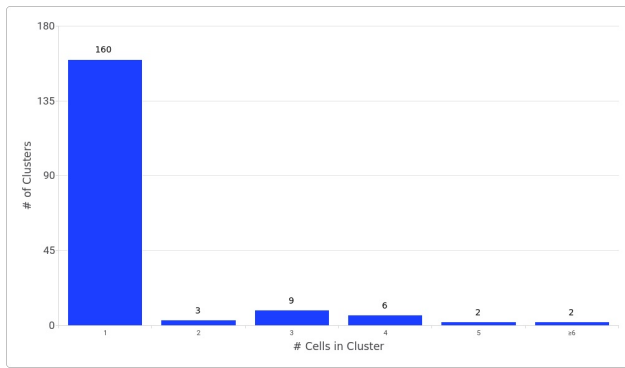

Cluster Size