

## Trypan Blue Tissue Culture

---

|                   |                    |                    |                            |
|-------------------|--------------------|--------------------|----------------------------|
| Sample Name:      | <b>Sample Name</b> | Created Date/Time: | <b>2026-01-23 10:50:51</b> |
| Account:          | <b>General</b>     | Passage:           |                            |
| Software Version: | <b>v4.3.4</b>      | Firmware Version:  | <b>11.66</b>               |
| Instrument SN:    | <b>s-07097</b>     | Record:            | <b>20260123105051</b>      |
| Description:      |                    |                    |                            |

## Results

---

|                           |                            |                           |                 |
|---------------------------|----------------------------|---------------------------|-----------------|
| Last Processed Date/Time: | <b>2026-01-23 10:50:51</b> | Gating Min Diameter (um): | <b>4</b>        |
| Gating Max Diameter (um): | <b>20</b>                  | Live Cell Count:          | <b>223</b>      |
| Dead Cell Count:          | <b>561</b>                 | Total Cell Count:         | <b>784</b>      |
| % Viability:              | <b>28.4439</b>             | Mean Diameter (um):       | <b>13.04</b>    |
| Live Cells/mL:            | <b>1.31e+06</b>            | Dead Cells/mL:            | <b>3.30e+06</b> |
| Total Cells/mL:           | <b>4.61e+06</b>            |                           |                 |

## Dilution

---



|                     |            |                         |            |
|---------------------|------------|-------------------------|------------|
| Target Cells/mL:    | <b>N/A</b> | Target Number of Cells: | <b>N/A</b> |
| Target Volume (mL): | <b>0</b>   | Original Volume (mL):   | <b>0</b>   |
| Dilution Guidance:  |            |                         |            |

## Protocol





---


|                             |              |                             |                |
|-----------------------------|--------------|-----------------------------|----------------|
| Protocol:                   | <b>Scm</b>   | DirectPipette (or Slide):   | <b>Pipette</b> |
| Chamber Height:             | <b>100</b>   | Dilution Factor:            | <b>2</b>       |
| Protocol Min Diameter (um): | <b>4</b>     | Protocol Max Diameter (um): | <b>20</b>      |
| Live Roundness:             | <b>35</b>    | Dead Roundness:             | <b>15</b>      |
| Stained Threshold:          | <b>5</b>     |                             |                |
| Small Cell Mode:            | <b>True</b>  |                             |                |
| Irregular Cell Mode:        | <b>False</b> |                             |                |

## Sample Images

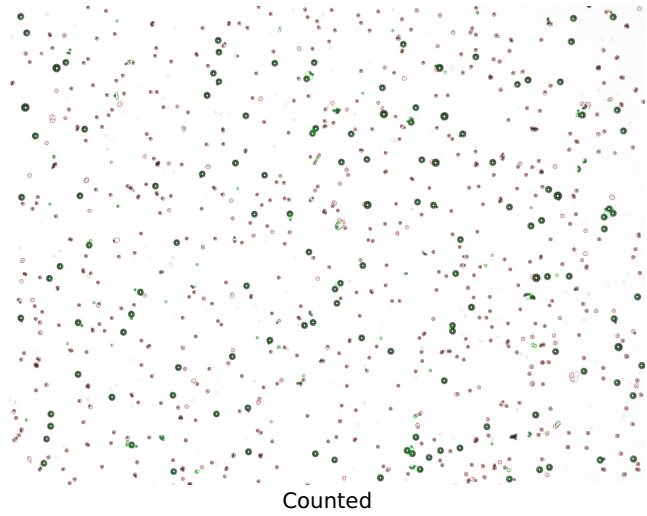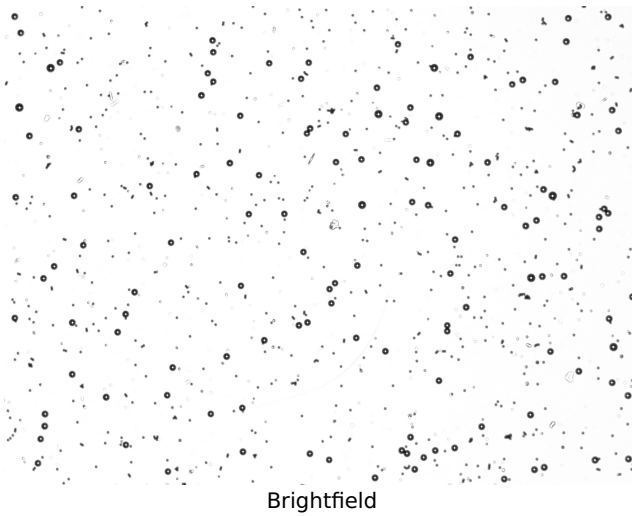

## Sample Histograms

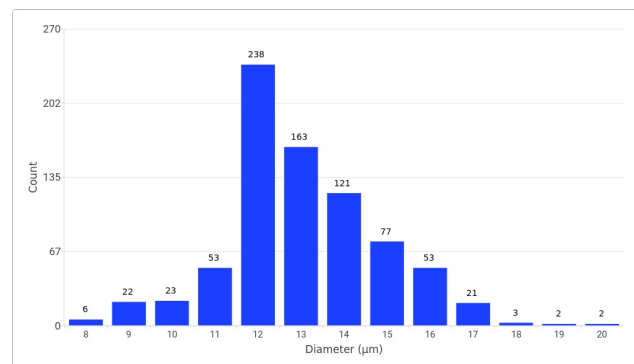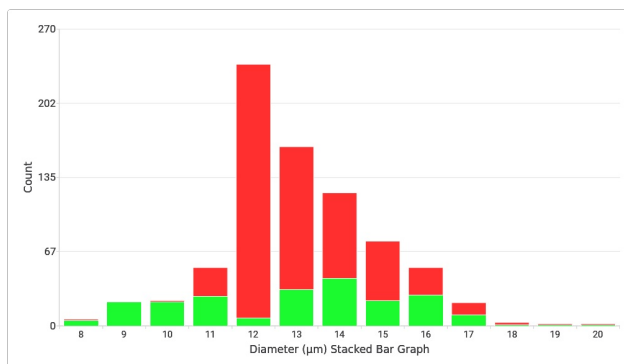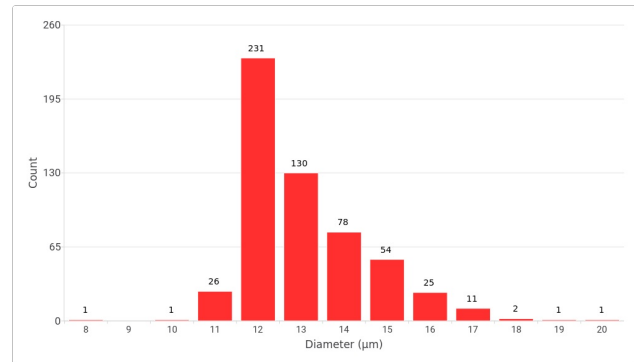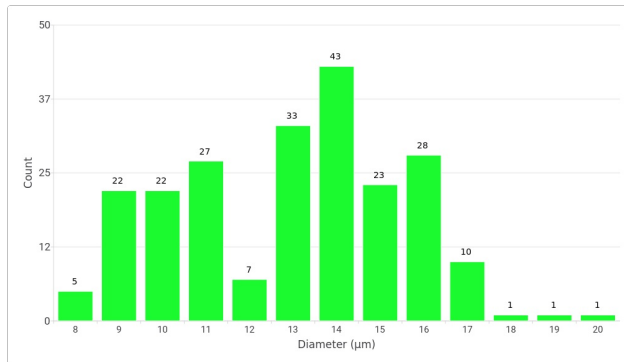

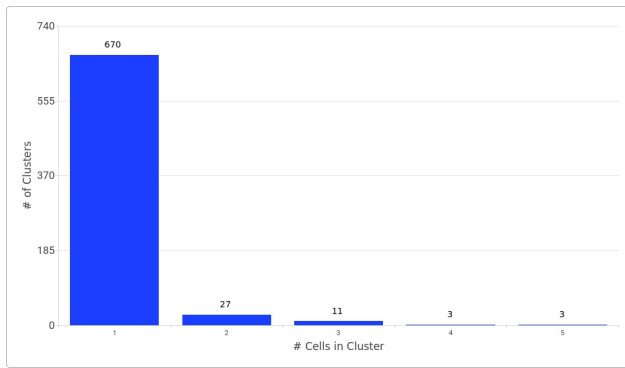

Cluster Size