

Trypan Blue Tissue Culture

Sample Name:	Sample Name	Created Date/Time:	2024-11-15 10:05:14
Account:	General	Passage:	
Software Version:	v4.1.0	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20241115100514
Description:			

Results

Last Processed Date/Time:	2024-11-15 10:12:40	Gating Min Diameter (um):	10
Gating Max Diameter (um):	20	Live Cell Count:	614
Dead Cell Count:	93	Total Cell Count:	707
% Viability:	86.8458	Mean Diameter (um):	15.84
Live Cells/mL:	3.61e+06	Dead Cells/mL:	5.47e+05
Total Cells/mL:	4.16e+06		



Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			





Protocol


Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	2
Protocol Min Diameter (um):	10	Protocol Max Diameter (um):	20
Live Roundness:	90	Dead Roundness:	25
Stained Threshold:	20		
Small Cell Mode:	False		
Irregular Cell Mode:	False		

Sample Images

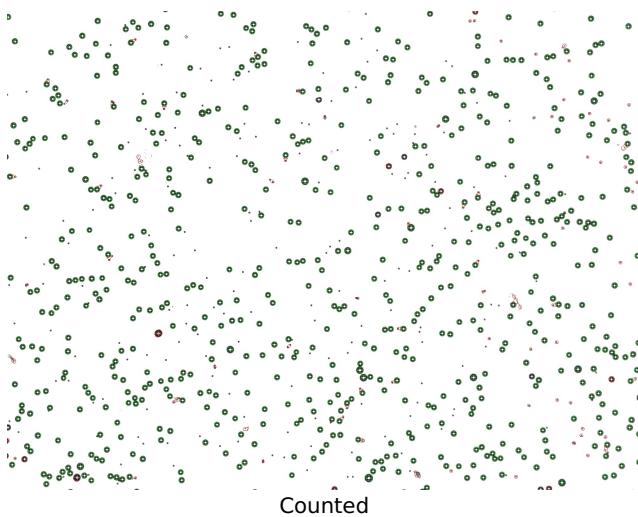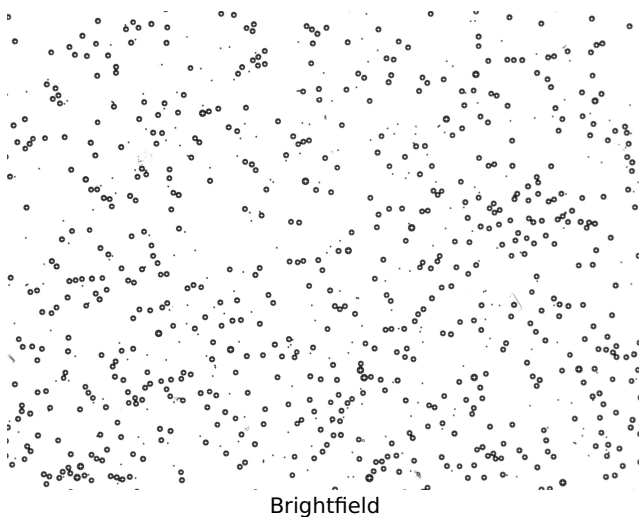

Sample Histograms

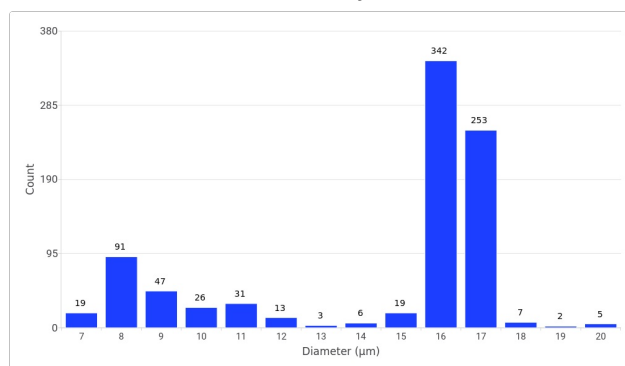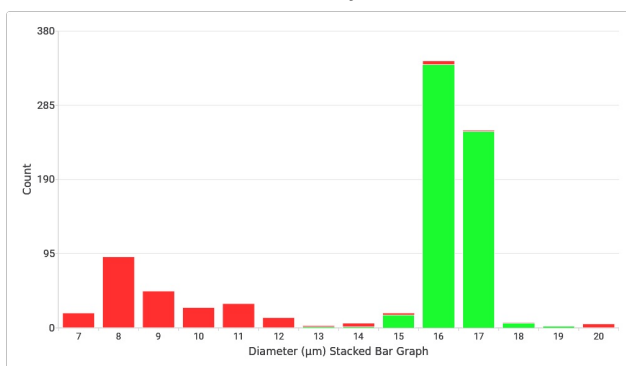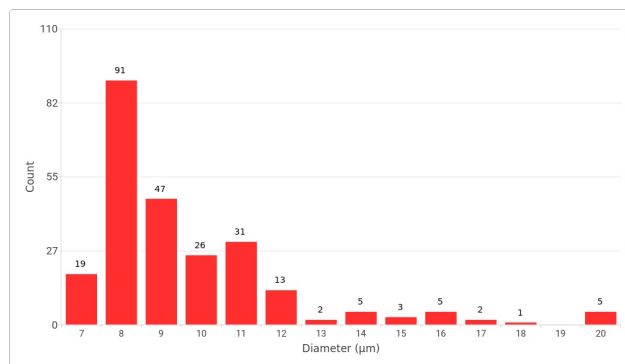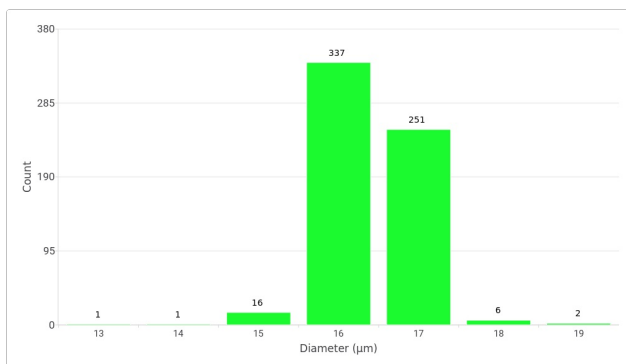

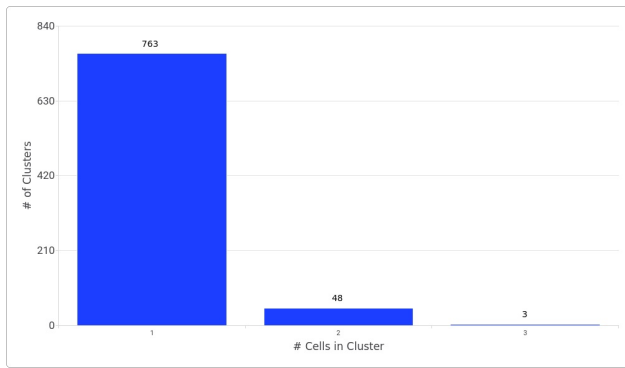

Cluster Size