

Yeast

Sample Name:	Sample Name	Created Date/Time:	2024-07-02 10:46:29
Account:	General	Passage:	
Software Version:	v4.0.0	Firmware Version:	11.66
Instrument SN:	s-07097	Record:	20240702104629
Description:			

Results

Last Processed Date/Time:	2024-07-02 10:46:29	Gating Min Diameter (um):	2
Gating Max Diameter (um):	10	Live Cell Count:	7
Dead Cell Count:	12	Total Cell Count:	19
% Viability:	36.8421	Mean Diameter (um):	8.94
Live Cells/mL:	2.28e+04	Dead Cells/mL:	3.92e+04
Total Cells/mL:	6.20e+04		


Dilution

Target Cells/mL:	N/A	Target Number of Cells:	N/A
Target Volume (mL):	0	Original Volume (mL):	0
Dilution Guidance:			


Protocol

Protocol:	Default Protocol	DirectPipette (or Slide):	Pipette
Chamber Height:	100	Dilution Factor:	1.11
Protocol Min Diameter (um):	2	Protocol Max Diameter (um):	10
Live Roundness:	1	Dead Roundness:	1
Green Fluorescence Threshold:	1	Red Fluorescence Threshold:	1
Irregular Cell Mode:	False		

Sample Images

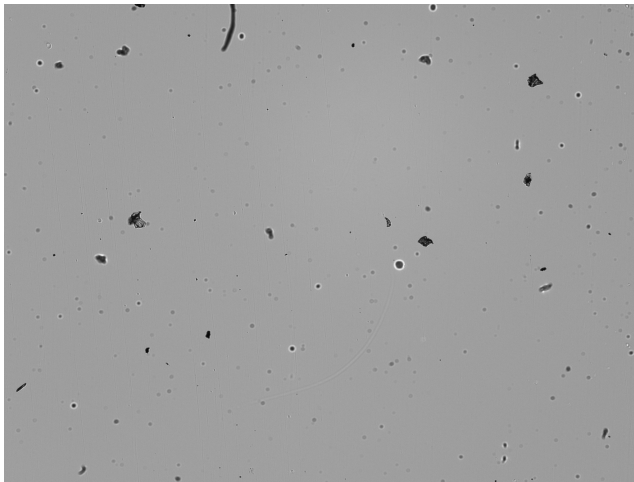


Brightfield

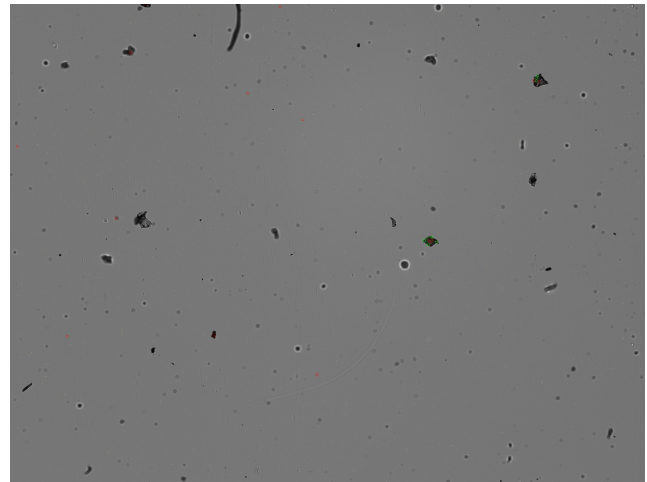


Counted


Sample Histograms

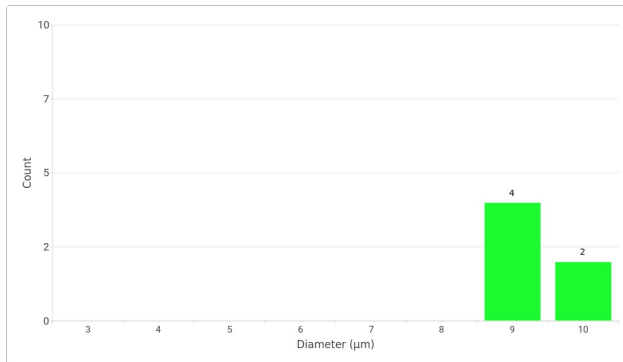


Live Cells (by Size)

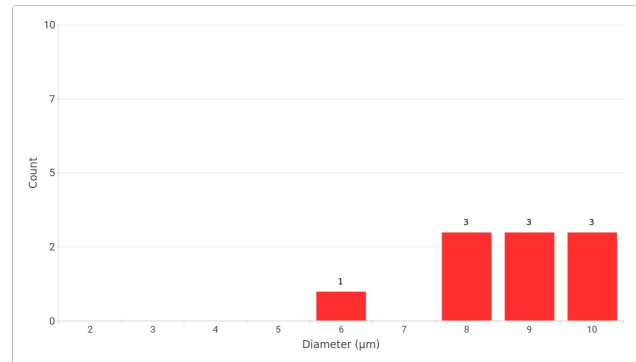


Dead Cells (by Size)

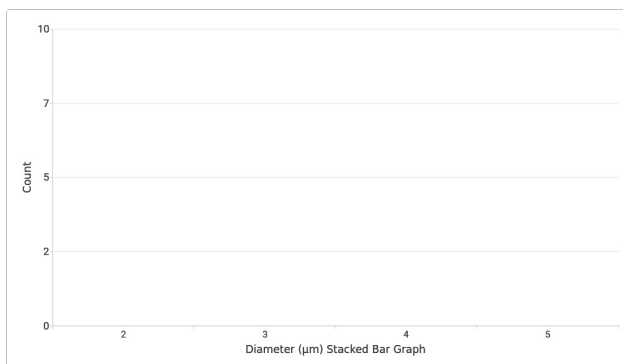

Live+Dead Cells (by Size)

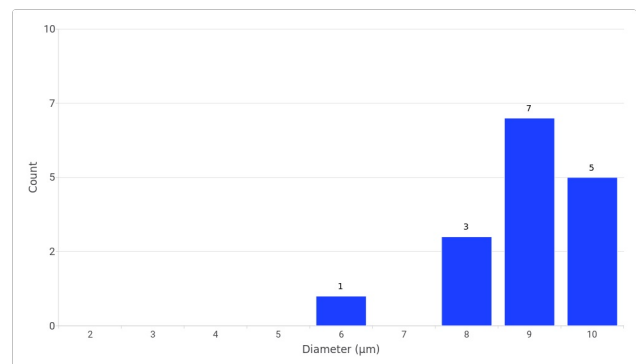

Total Cells (by Size)

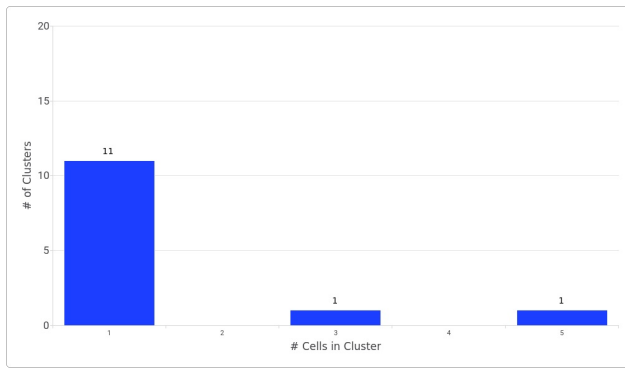

Cluster Size