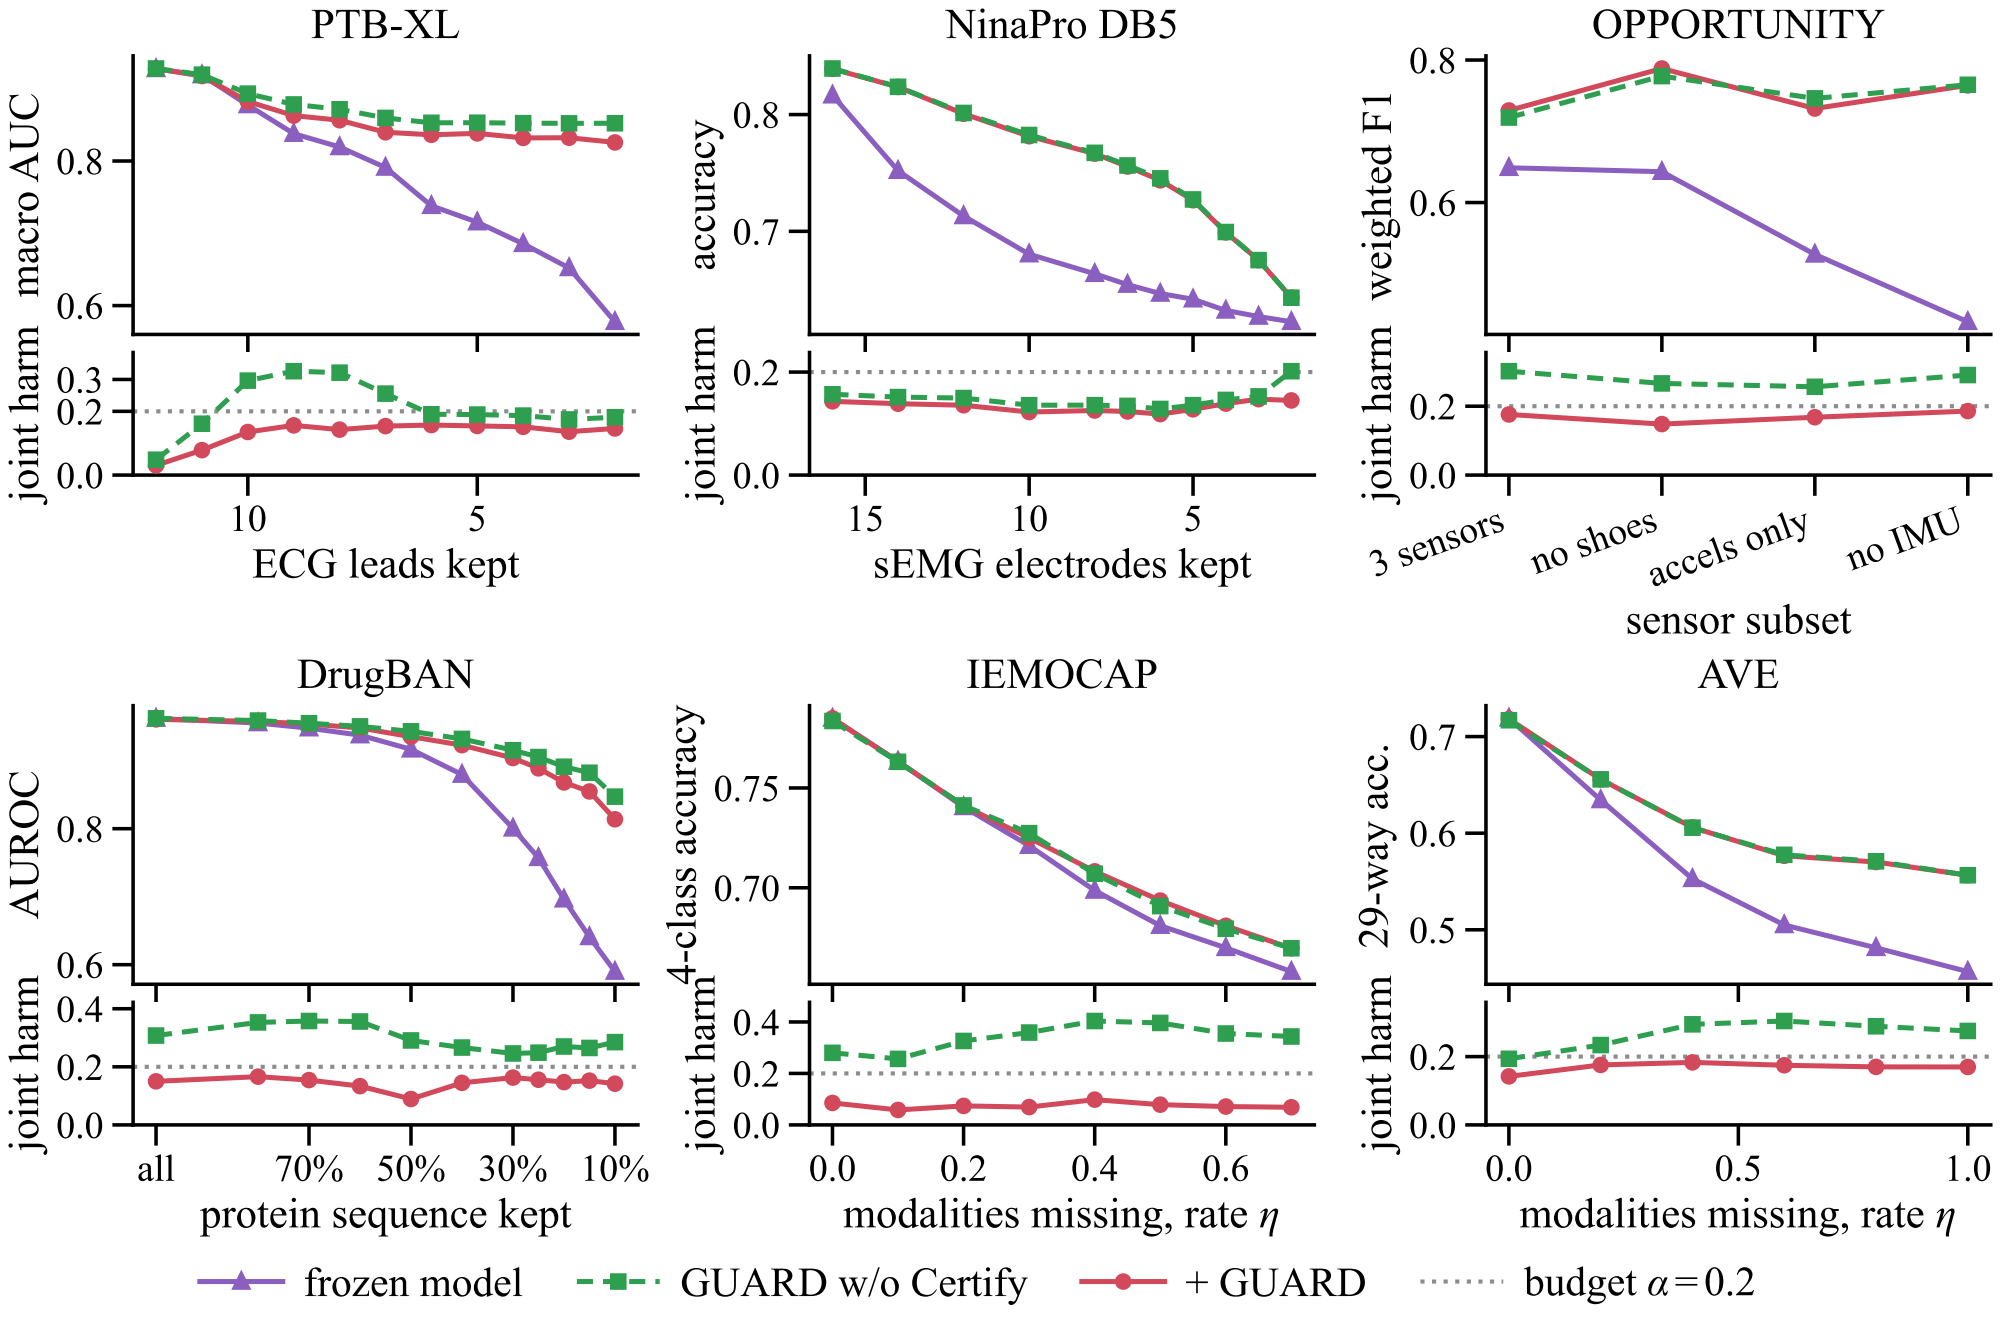
PTB-XL
NinaPro DB5
OPPORTUNITY
macro AUC
accuracy
weighted F1
joint harm
ECG leads kept
sEMG electrodes kept
3 sensors
no shoes
accels only
no IMU
sensor subset
DrugBAN
IEMOCAP
AVE
AUROC
4-class accuracy
29-way acc.
all
70%
50%
30%
10%
protein sequence kept
modalities missing, rate η
frozen model
GUARD w/o Certify
+ GUARD
budget α = 0.2