

Computer Name: LENOVO-PC3


User Name: Admin

Time stamp: 12/3/2018 11:15:51 AM

CH0 Real



LabVIEW

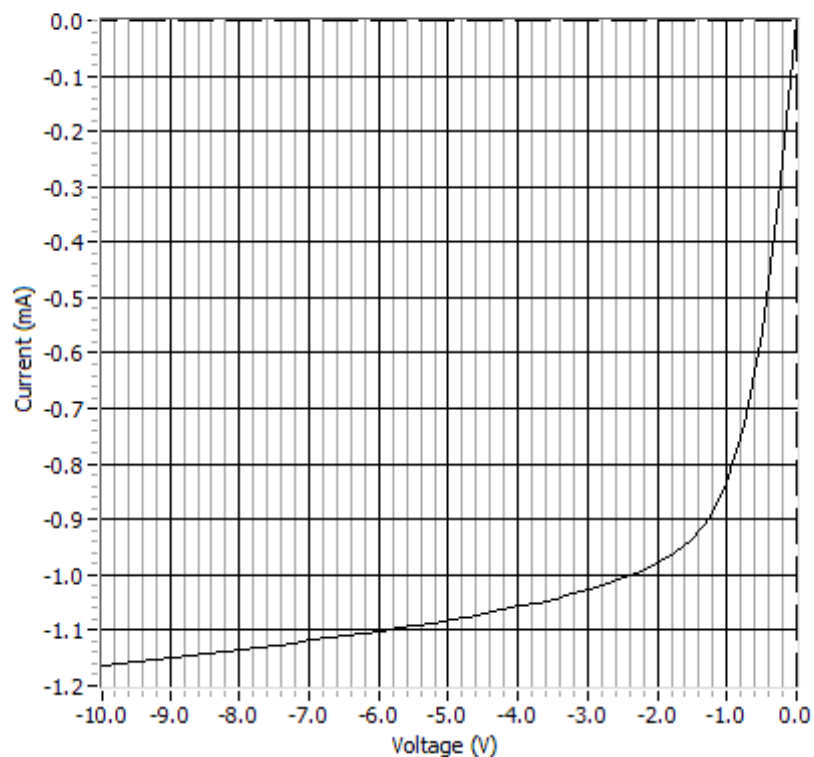

Current (mA) -0.00

Voltage (V) 0.00

| Parameter | Value |
|------------------------|--------------------|
| Device | Dev1 (NI ELVIS II) |
| Start Voltage | -10.00 V |
| Increment Voltage | 0.25 V |
| Stop Voltage | 0.00 V |
| Current Negative Limit | -40.00 mA |
| Current Positive Limit | 40.00 mA |
| Gain | Low |
| Voltage Scale | Linear |
| Current Scale | Linear |