

Computer Name: LENOVO-PC2

User Name: Admin

Time stamp: 05-Nov-18 11:16:34 AM


CH0 Real



CH1 Real



Sample Rate: 250.00 kS/s

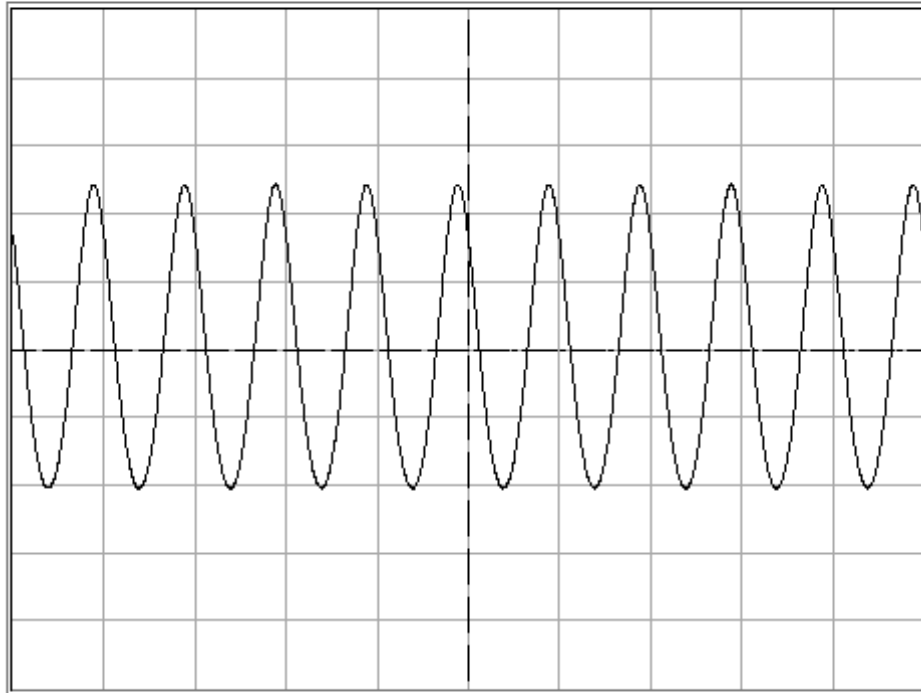

Timeout

CH0 Meas: RMS: 31.46 mV Freq: 1.000 kHz Vp-p: 89.92 mV

Channel Settings	Channel 0 Values
Source	SCOPE CH 0
Probe	1x
Coupling	AC
Volts / Div (V)	20 mV
Vertical Position (Div)	0 (Div)
Parameter	Value
Device	Dev4 (NI ELVIS II)
Time Base (s)	1 ms
Trigger Type	Immediate