



Hg calibration fit: 404.770 nm line, Gaussian + linear background

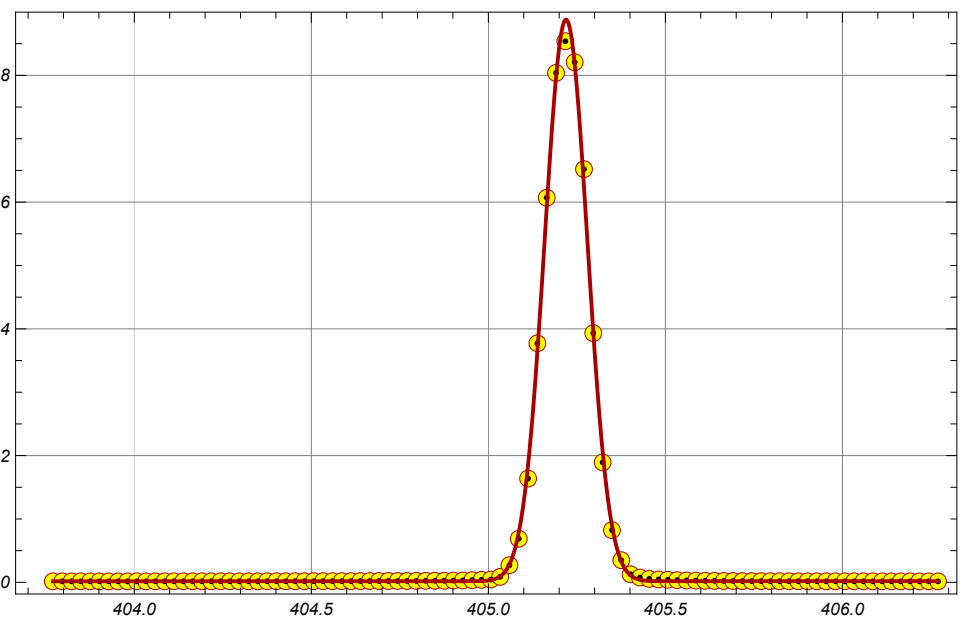

Residuals and Effective Uncertainties

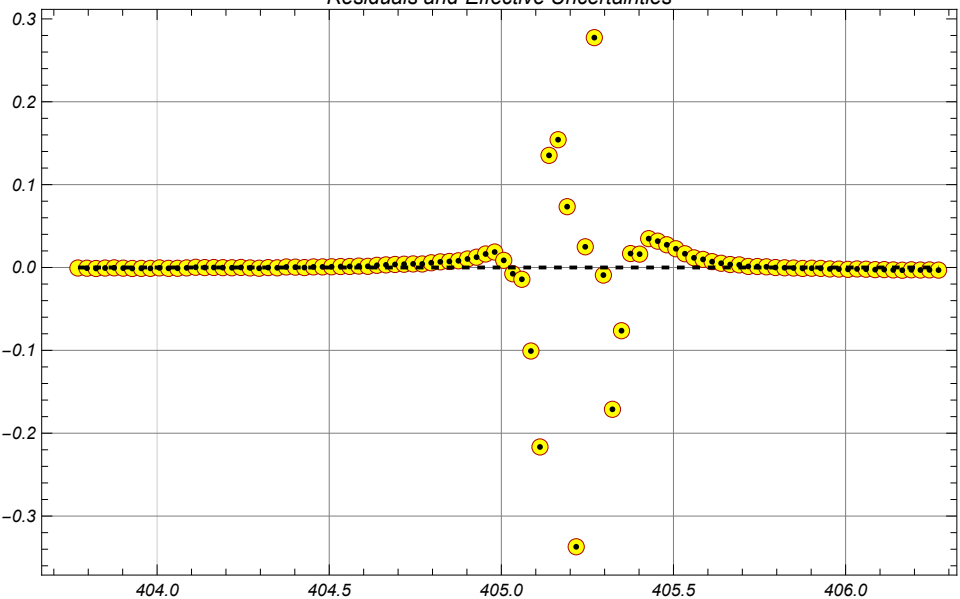

$$y(x) = y_{\max} \exp\left(\frac{-(x-\mu)^2}{2\sigma^2}\right) + c + d(x - \mu)$$

c= 0.0178177 d= 0.000792837

σ_c = 0.00712897 σ_d = 0.0086559

$y_{\max}$ = 8.8619 μ = 405.219 sigma= 0.0603832

$\sigma_{y_{\max}}$ = 0.0369959 σ_{μ} = 0.000290299 σ_{sigma} = 0.000290438 Std. deviation= 0.060868