



# Hg calibration scan: 405.0 nm region

*Before conversion: instrument wavelength (2nd order)*

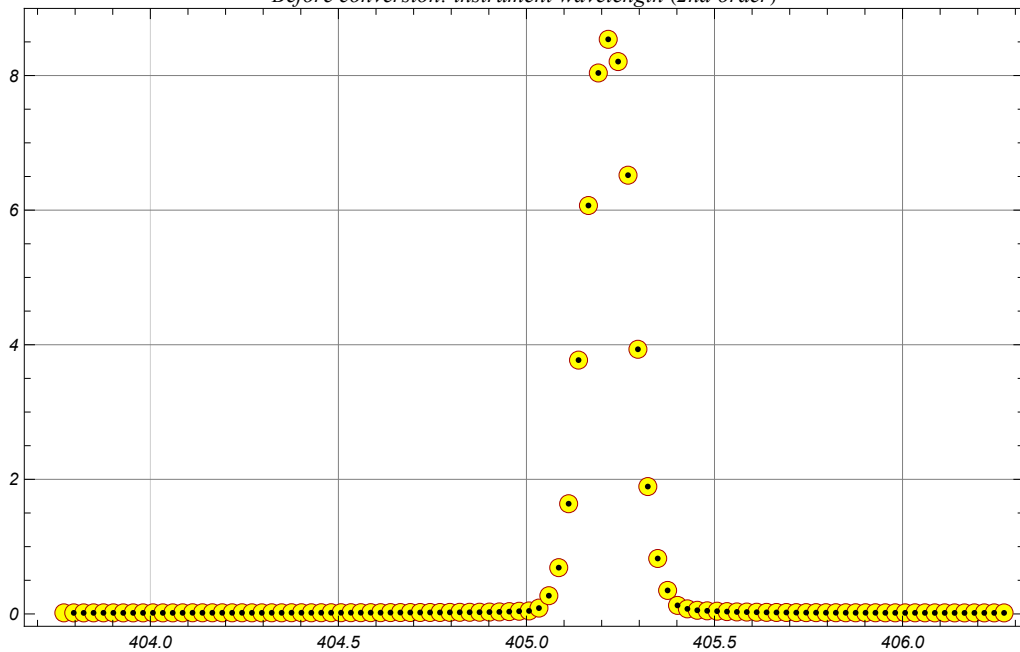

*After conversion: real wavelength = instrument wavelength / 2*

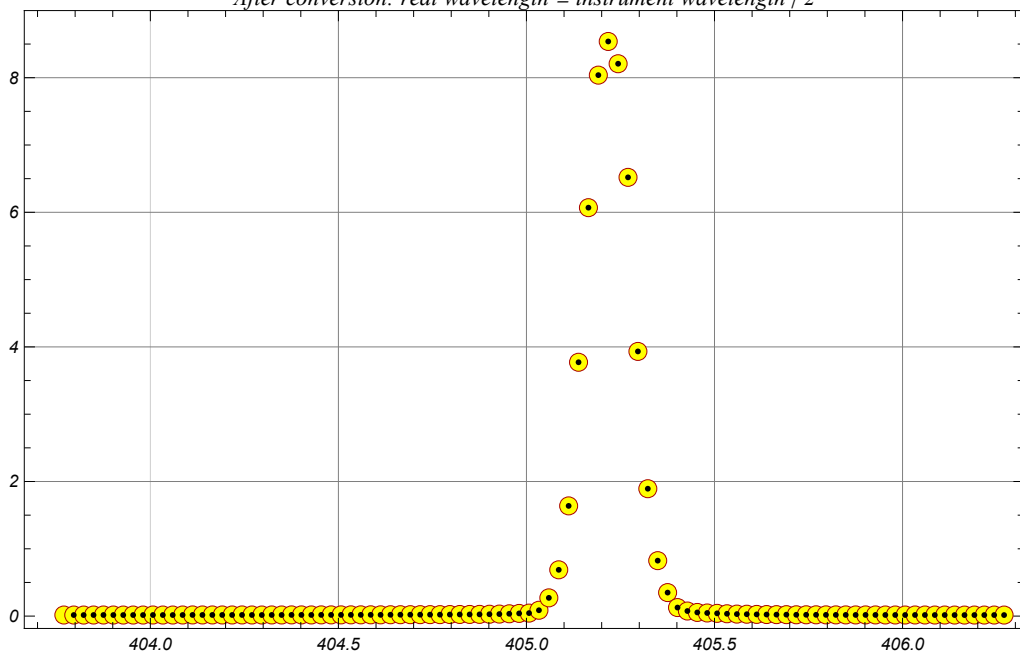

Top panel: before conversion (instrument wavelength, 2nd order). Bottom panel: after conversion (real wavelength = instrument wavelength / 2).