



Hg calibration scan: 546.3 nm region

Before conversion: instrument wavelength (2nd order)

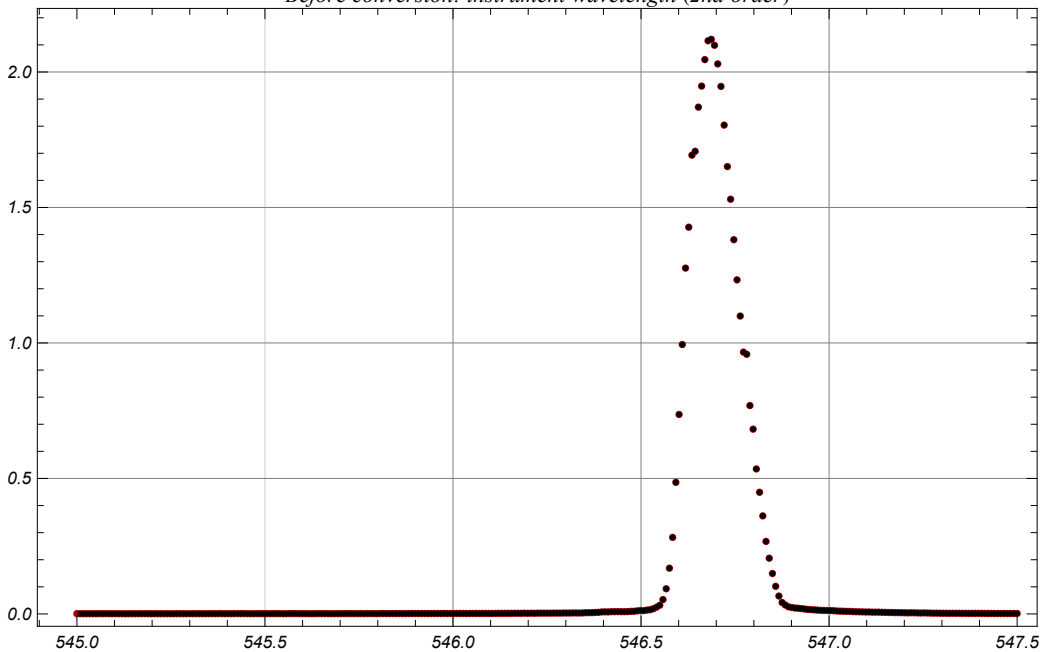

After conversion: real wavelength = instrument wavelength / 2

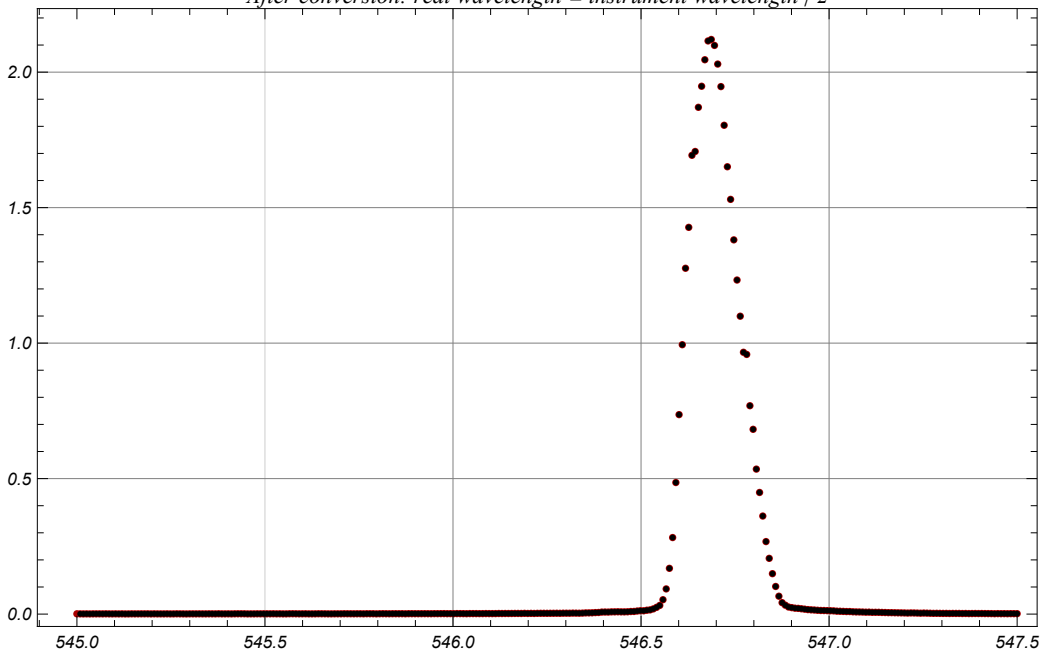

Top panel: before conversion (instrument wavelength, 2nd order). Bottom panel: after conversion (real wavelength = instrument wavelength / 2).