
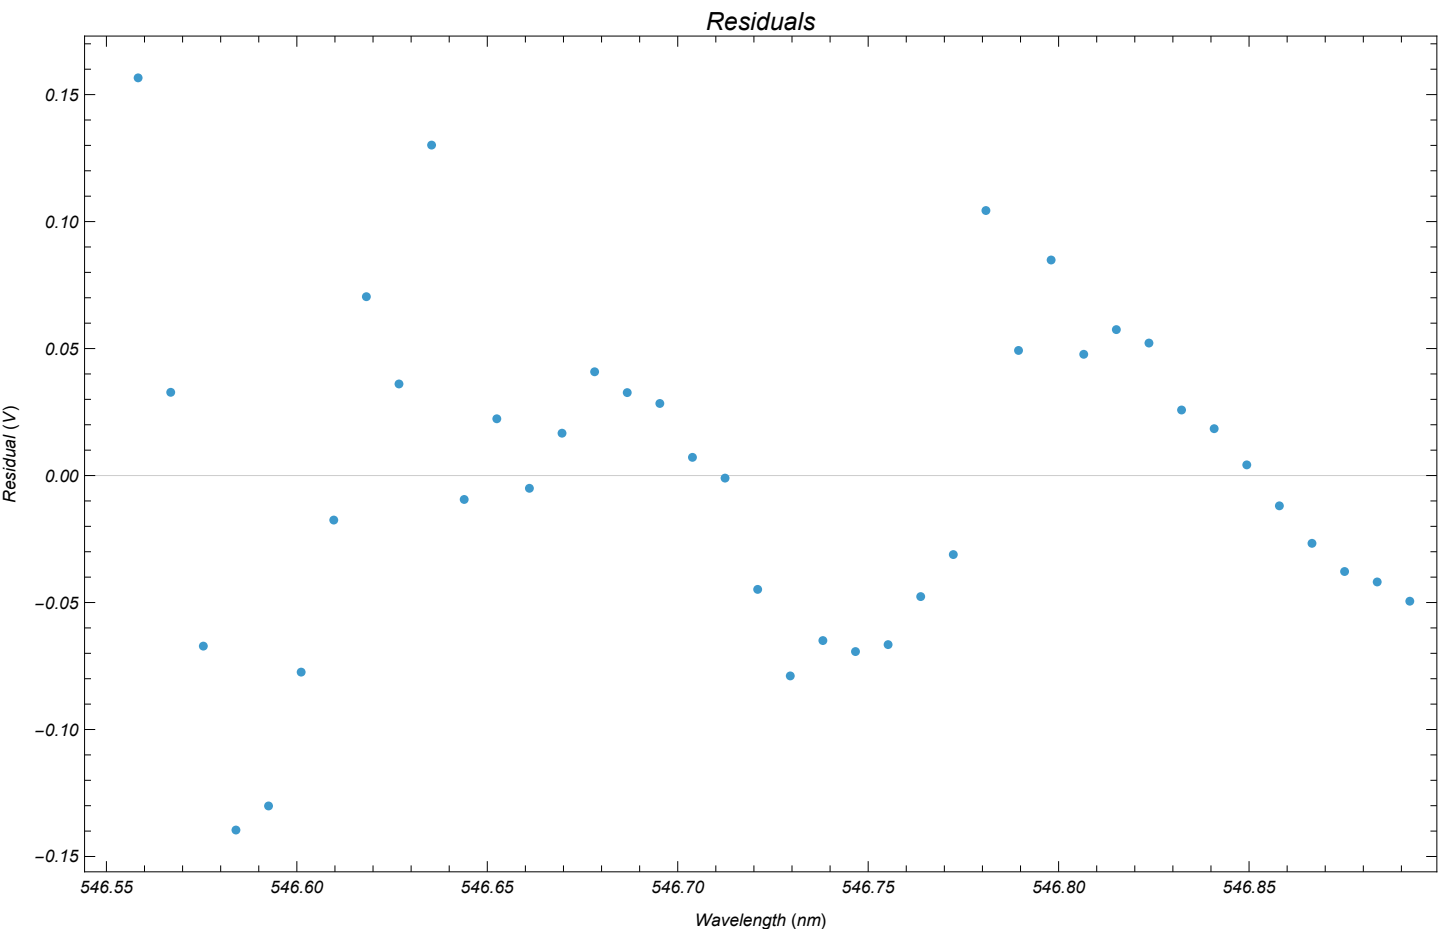


Native Mathematica fitreport: Hg 546 repeat 20um

File: 15_Hg_calibration_546.250nm_same_data_as_562hg_2nm_scan_but_slit_width_is_20_nm_REAL_FOR_CURVEFIT.dat

Fit window: {546.55, 546.9} nm

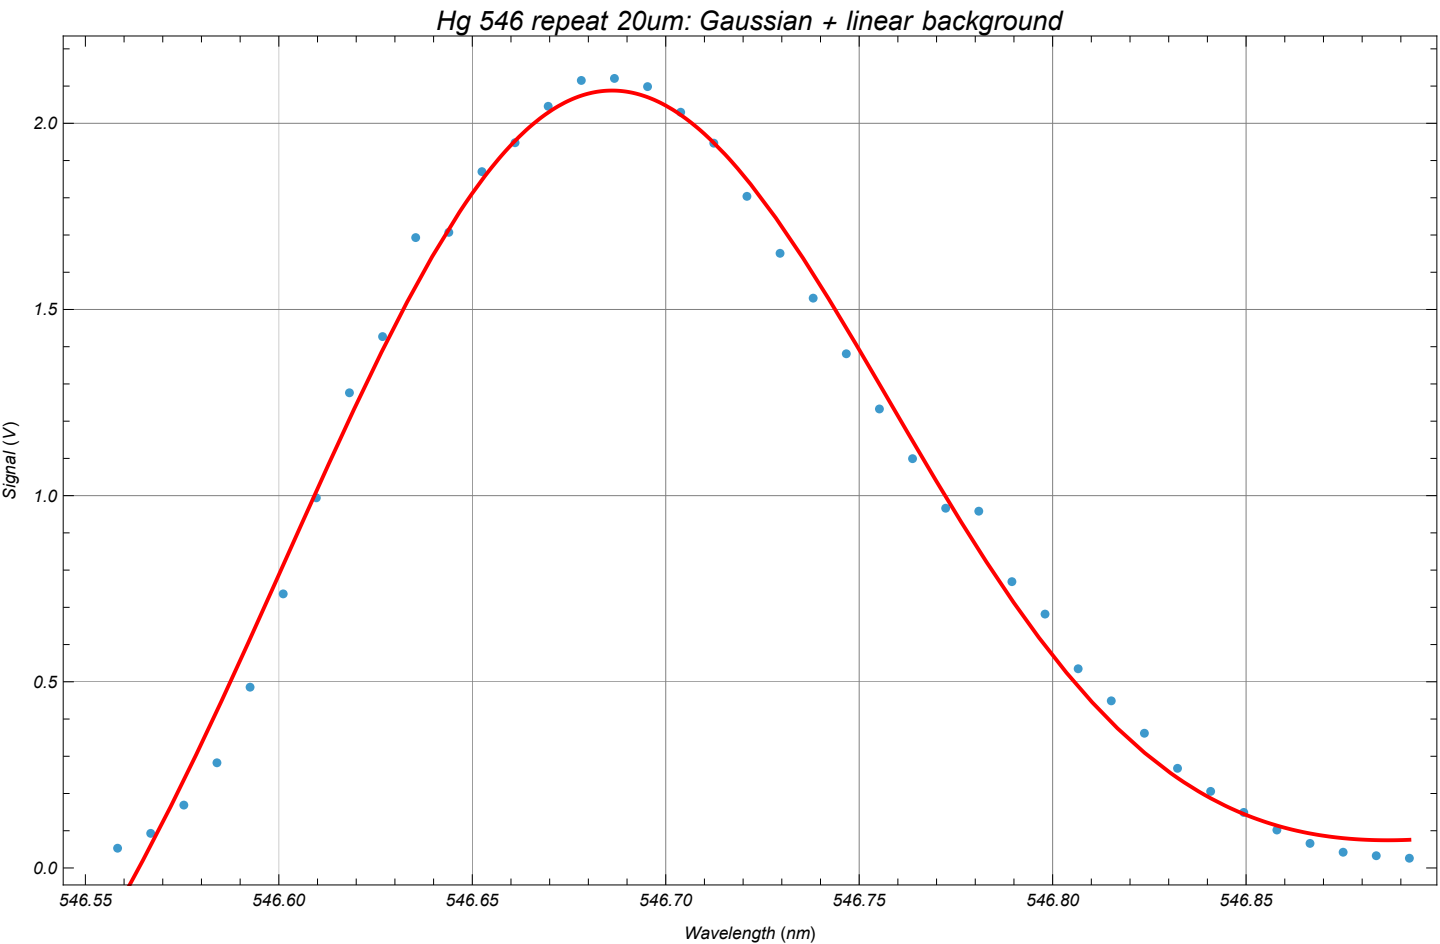

parameter	estimate	standard error
c	-0.438991	0.0941349
d	2.69115	0.437428
amp	2.64063	0.107734
mu	546.68	0.00202291
sigma	0.0780507	0.00286805
RMS residual	0.0635922	
max residual	0.156594	
true Hg wavelength	546.226	
used for calibration?	False	